# Technical Information **Prosonic S FDU92**

Ultrasonic measuring technology



## Ultrasonic sensor for level measurement and flow measurement

#### Application

- Continuous, non-contact level measurement of liquids and bulk solids in silos, on conveyor belts, in material stockpiles and in crushers
- Flow measurement in open flumes and measuring weirs
- Maximum measuring range: 20 m (66 ft) in liquids; 10 m (33 ft) in bulk solids

#### Your benefits

- Integrated temperature sensor for time-of-flight correction, enabling accurate measurements even if temperatures change
- Hermetically welded PVDF sensor for maximum chemical resistance
- Suitable for harsh ambient conditions thanks to separate transmitter installation (up to 300 m (984 ft))
- Self-cleaning effect ensures minimum deposit build-up
- Weather resistant and flood-proof (IP68)
- International Dust-Ex and Gas-Ex certificates available

### Table of contents

Document conventions	
Function and system design	4
Input	5 . 5
Power supply  Supply voltage  Electrical connection  Connection diagram for sensor → FMU90  Connection diagram for sensor → FMU95  Extension cable specifications  Shortening the sensor cable	6 6 6 7 7
Installation Installation conditions for level measurement Installation conditions for flow measurement Installation options (examples) Nozzle mounting Ultrasound guide pipe for measurement in narrow pits Securing the sensor	. 8 8
Environment  Degree of protection  Vibration resistance  Storage temperature  Thermal shock resistance  Electromagnetic compatibility	11 11 11 11 11 11
Process	<b>12</b> 12 12
Mechanical construction  Dimensions  Dimensions of G1" counter nut  Weight  Materials  Materials of connecting cable  Material of G1" counter nut	12 12 12 12 13 13
Certificates and approvals  CE mark  RoHS  RCM-Tick marking  Ex approval  Other standards and guidelines	13 13 13 13 13 13

Ordering information	14
Ordering information	14
5-point linearity protocol	14
Scope of delivery	15
Accessories	15
Sensor extension cable	
Screw-in flange FAX50	15
Cantilever arm for the sensors	15
Mounting bracket for ceiling mounting	19
FAU40 alignment unit	19
IP66 protective housing for RNB130 power supply unit	20
Supplementary documentation	20
Documentation for FMU90 transmitter	20
Documentation for FMU95 transmitter	21
Other documentation	2.1

### Important document information

#### **Document conventions**

#### Safety symbols

⚠ DANGER
This symbol alerts you to a dangerous situation. Failure to avoid this situation will result in serious or fatal injury.

#### **WARNING**

This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in serious or fatal injury.

This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.

#### **NOTICE**

This symbol contains information on procedures and other facts which do not result in personal injury.

#### **Electrical symbols**



Ground connection

A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.

#### Tool symbols



Open-ended wrench

#### Symbols for certain types of information and graphics

Procedures, processes or actions that are permitted

#### **K** Forbidden

Procedures, processes or actions that are forbidden

Indicates additional information

Reference to documentation

#### 1., 2., 3.

Series of steps

#### 1, 2, 3, ...


Item numbers

#### A, B, C, ...

Views

### Function and system design

#### Level measurement

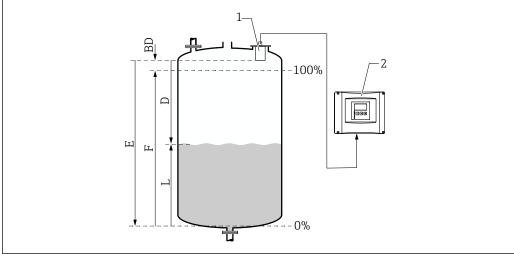

A0034882


- 1 Prosonic S sensor
- 2 Prosonic S transmitter
- BD Blocking distance
- D Distance between reference point (sensor membrane) and surface of medium
- E Empty distance
- F Span
- L Level

The sensor transmits ultrasonic pulses in the direction of the surface of the medium. There, they are reflected back and received by the sensor. The transmitter measures the time t between the transmission and reception of a pulse. From this time, and using the sonic velocity c, the transmitter calculates the distance D between the reference point (sensor membrane) and the surface of the medium:

 $D = c \cdot t/2$ 

The level L is derived from D. With linearization, the volume V or the mass M is derived from L.

### Flow measurement in flumes or weirs

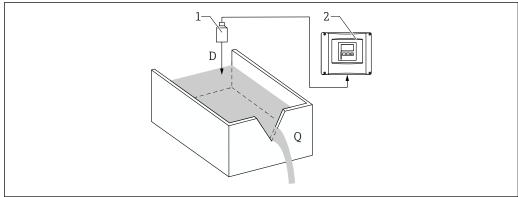

A003521

- 1 Prosonic S sensor
- 2 Prosonic S transmitter
- D Distance between sensor membrane and surface of liquid
- Q Flow

The sensor transmits ultrasonic pulses in the direction of the surface of the liquid. There, they are reflected back and received by the sensor. The transmitter measures the time t between the transmission and reception of a pulse. From this time, and using the sonic velocity c, the transmitter calculates the distance D between the (reference point) sensor membrane and the surface of the liquid:

 $D = c \times t/2$ 

The level L is derived from D. With linearization, the flow Q is derived from L.


### Temperature-dependent time-of-flight correction

Temperature-dependent time-of-flight correction via the temperature sensors integrated in the ultrasonic sensors.

#### Input

#### Blocking distance

Signals within the blocking distance (BD) range cannot be measured due to the transient response of the sensor.

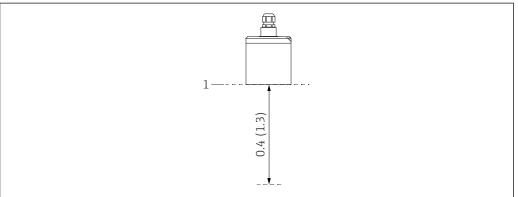

4002070

- $\blacksquare$  1 Blocking distance of the ultrasonic sensor. Engineering unit m (ft)
- 1 Reference point (sensor membrane) of measurement

#### Measuring range

#### Estimation of the effective sensor range depending on the operating conditions

- 1. Add up all the applicable attenuation values from the following lists.
- 2. From the total calculated attenuation, use the range chart below to calculate the range of the sensor.

#### Attenuation caused by surface of liquid

- Calm surface: 0 dB
- Waves on surface: 5 to 10 dB
- Very turbulent surface: 10 to 20 dB
- Frothy surface: contact Endress+Hauser: http://www.endress.com/contact

#### Attenuation due to bulk solids surface

- Hard, rough surface (e.g. rubble): 40 dB
- Soft surface (e.g. peat, dust-covered clinker): 40 to 60 dB

#### Attenuation due to dust


- No dust formation: 0 dB
- Minor dust formation: 5 dB
- Major dust formation: 5 to 20 dB

#### Attenuation caused by filling curtain in detection range

- No filling curtain: 0 dB
- Small volumes: 5 dB
- Large volumes: 5 to 20 dB

#### Attenuation caused by temperature difference between sensor and product surface

- Up to 20 °C (68 °F): 0 dB
- Up to 40 °C (104 °F): 5 to 10 dB
- Up to 80 °C (176 °F): 10 to 20 dB

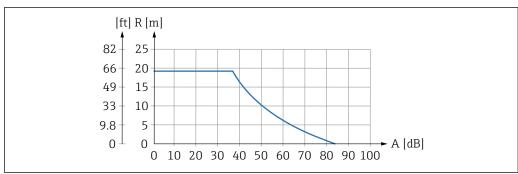

- **₽** 2 Range chart for ultrasonic sensors
- Total attenuation in dB
- R Range in m (ft)

#### Operating frequency

30 kHz

### **Power supply**

Supply voltage

Is provided by the transmitter.

#### **Electrical connection**

#### General information

#### **NOTICE**

#### Interference signals may cause malfunctions


Do not route the sensor cables parallel to high-voltage electric power lines or near frequency converters.

#### NOTICE

#### A damaged cable shield may cause malfunctions


- For pre-terminated cables: connect the black wire (shield) to the "BK" terminal.
- For extension cables: twist the shield and connect to the "BK" terminal.

#### Connection diagram for sensor → FMU90

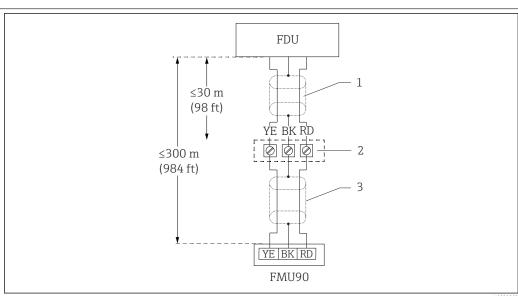

- **₽** 3 Connection diagram for sensor; YE: yellow, BK: black; RD: red; BU: blue; BN: brown; protective conductor GNYE: green/yellow
- Shielding of sensor cable
- Terminal box 2
- Shielding of extension cable

### Connection diagram for sensor → FMU95

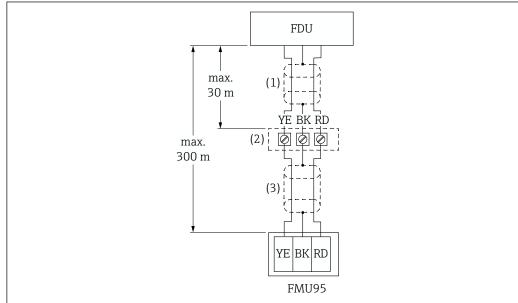

. . . . . . . . .

- Connection diagram for sensor; YE: yellow, BK: black; RD: red; BU: blue; BN: brown; protective conductor GNYE: green/yellow
- 1 Shielding of sensor cable
- 2 Terminal box
- 3 Shielding of extension cable

## Extension cable specifications

### Maximum total length (sensor cable + extension cable)

300 m (984 ft)

Number of wires

As per connection diagram

Shielding

One shielding braid for the YE wire and one for the RD wire (no foil shield)

Cross-section

0.75 to 2.5 mm<sup>2</sup> (18 to 14 AWG)

Resistance

Max.  $8 \Omega$  per wire

Capacitance, wire to shield

Max. 60 nF




Suitable extension cables are available from Endress+Hauser.

#### Shortening the sensor cable

The sensor cable can be shortened if necessary (see the Operating Instructions for the FMU90 or FMU95 transmitter).

#### Installation

### Installation conditions for level measurement

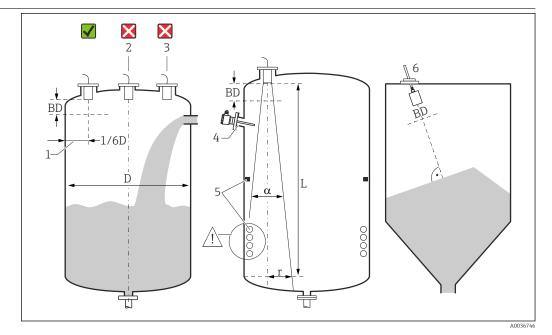

■ 5 Installation conditions for level measurement

- 1 Recommended distance to the vessel wall: 1/6 of the vessel diameter D.
- 2 Do not mount in the center of the vessel.
- 3 Avoid measurements through the filling curtain.
- 4 There must be no internal fixtures in the signal beam.
- 5 Symmetrical internal fixtures, in particular, negatively impact the measurement.
- 6 For bulk solids: using the FAU40 alignment unit, align the sensor so that it is perpendicular to the surface of the product.
- BD Blocking distance

#### Emitting angle/beam

- α (typical) = 11°
- L (max) = 20 m (66 ft)
- r (max) = 1.92 m (6.3 ft)

#### Other conditions

- The lower edge of the sensor should be located inside the vessel
- The maximum level may not enter the blocking distance

#### Several sensors in one vessel


Sensors that are connected to a common FMU90 or FMU95 transmitter can be used in one vessel.

## Installation conditions for flow measurement

#### Conditions

- ullet Mount the sensor on the upstream side above the maximum upstream level  $H_{max}$  plus the blocking distance BD
- Position the sensor in the center of the channel or weir
- Align the sensor so that it is perpendicular to the surface of the water
- Observe the specified mounting distance (clearance) to the flume constriction or weir edge See the Operating Instructions for FMU90 / FMU95
- Protect the sensor against sun and precipitation using the weather protection cover

#### Example: Khafagi-Venturi flume

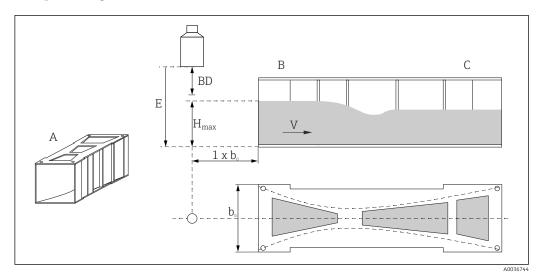


- Khafagi-Venturi flume
- Width of Khafagi-Venturi flume  $b_0$
- В Upstream side
- С Downstream side
- Blocking distance of the sensor
- Empty calibration (to be entered during commissioning)

 $H_{max}$  Maximum upstream level

Flow

#### Example: Triangular weir

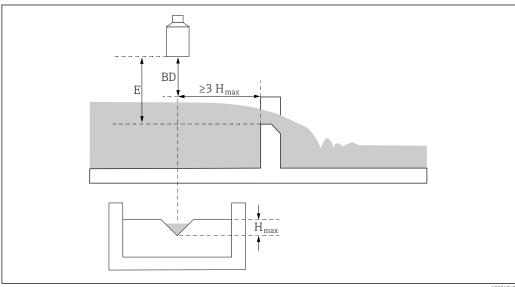


BD Blocking distance of the sensor

Empty calibration (to be entered during commissioning)


 $H_{max}$  Maximum upstream level

#### **Installation options** (examples)

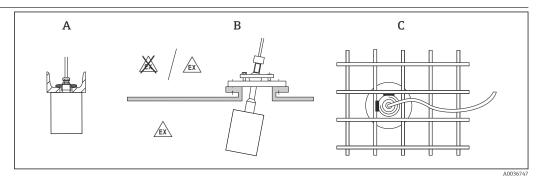

**₽** 6 Installation in systems


- Α On U-rail or bracket
- With FAU40 alignment unit В
- С With 1" sleeve welded to a grating

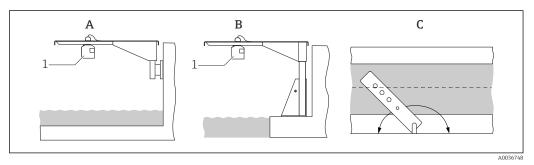

**₽** 7 Installation with cantilever arm over open channels or flumes

- Arm with wall bracket
- В Cantilever with mounting frame
- The arm can be turned (e.g. to position the sensor over the center of the channel)

#### Nozzle mounting

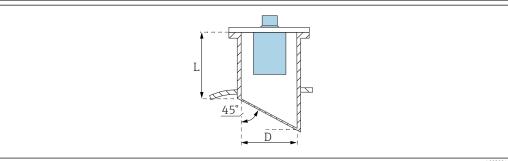

- D Nozzle diameter
- Nozzle length L


#### Conditions at the nozzle

- Smooth interior, without edges or welds
- No burr on the inside of the nozzle end on the tank side
- Beveled nozzle end on tank side (ideally: 45°)

#### Maximum nozzle length

D = DN150/6" to DN300/12":  $L_{max}$  = 400 mm (15.7 in)

## Ultrasound guide pipe for measurement in narrow pits

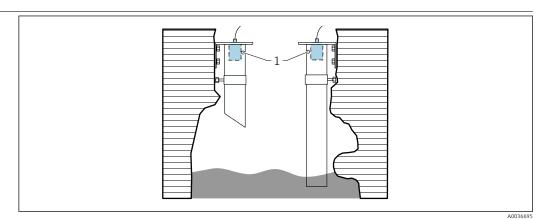

1 Venting hole


- Suitable ultrasound guide pipe: e.g. PE or PVC wastewater pipe
- Minimum diameter: DN200
- Venting hole at top
- No contamination from built-up dirt (clean regularly where necessary)

#### Securing the sensor

#### NOTICE

#### Risk of damage to the sensor

- ▶ Do not use the sensor cable for suspension purposes.
- ▶ Do not damage the sensor membrane when installing.

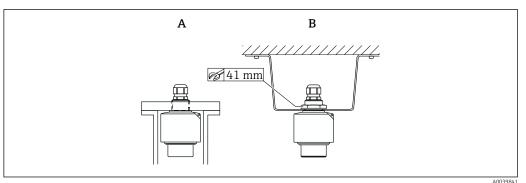

,

- 8 Securing the ultrasonic sensor
- A Mounted at rear thread
- B Mounted with counter nut

### **Environment**

Degree of protection	Tested according to IP68/NEMA6P (24 h at 1.83 m (6 ft) under water)
Vibration resistance	DIN EN 600068-2-64; 20 to 2000 Hz; 1 (m/s²)²/Hz; 3x100 min
Storage temperature	Identical to process temperature
Thermal shock resistance	Based on DIN EN 60068-2-14; test according to min./max. process temperature; 0.5 K/min; 1000 h
Electromagnetic compatibility	Electromagnetic compatibility in accordance with all the relevant requirements outlined in the EN 61326 series and NAMUR Recommendation EMC (NE 21). For details, refer to the Declaration of Conformity. With regard to interference emission, the devices meet the requirements of class A, and are only designed for use in an "industrial environment".

### **Process**

**Process temperature** 


- Non-Ex: -40 to +95 °C (-40 to +203 °F)
- Ex: -40 to +80 °C (-40 to +176 °F)

Process pressure

0.7 to 4 bar (10.15 to 58 psi)


### Mechanical construction

#### **Dimensions**

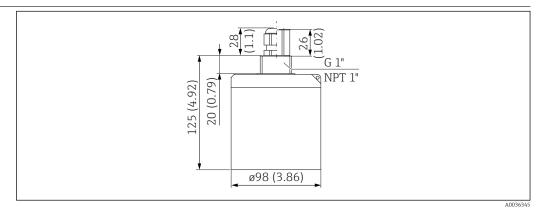

■ 9 Dimensions. Unit of measurement mm (in)

### Dimensions of G1" counter

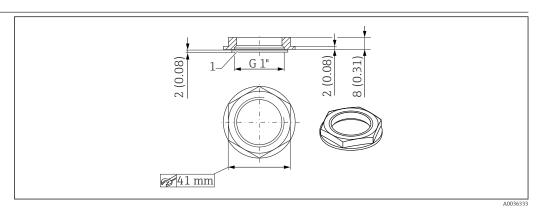

 $\blacksquare 10$  Counter nut; dimensions. Unit of measurement mm (in)

• The counter nut is included in the delivery for the following sensors: FDU92-\*G\*\* (rear G1 thread)


• The counter nut is not suitable for NPT threads.

Weight

Weight including cable 5 m (16 ft))

Approx. 2 kg (4.41 lb)

#### **Materials**

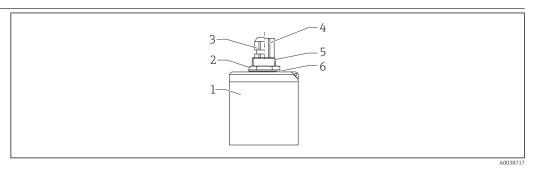

■ 11 Materials

- 1 Sensor housing: PVDF
- 2 Counter nut: PA6.6
- 3 Cable gland: PA
- 4 Pipe adapter: CuZn nickel-plated
- 5 O-ring: EPDM
- 6 Seal: EPDM

PVC

#### Materials of connecting cable

### Material of G1" counter nut

- Counter nut: PA6.6
- Seal (included in the delivery): EPDM

### Certificates and approvals

#### CE mark

The measuring system meets the legal requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied.

Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.

#### RoHS

The measuring system complies with the substance restrictions of the Restriction on Hazardous Substances Directive 2011/65/EU (RoHS 2).

#### **RCM-Tick marking**

The supplied product or measuring system meets the ACMA (Australian Communications and Media Authority) requirements for network integrity, interoperability, performance characteristics as well as health and safety regulations. Here, especially the regulatory arrangements for electromagnetic compatibility are met. The products are labelled with the RCM- Tick marking on the name plate.



A0029561

#### Ex approval

Available Ex approvals: see Product Configurator



Sensors with an Ex approval can be connected to the FMU90 transmitter without an Ex approval.

### Other standards and quidelines

#### EN 60529

Degrees of protection provided by enclosures (IP code)

#### EN 61326 series

EMC product family standard for electrical equipment for measurement, control and laboratory use

#### **NAMUR**

User association of automation technology in process industries

### **Ordering information**

#### Ordering information

Detailed ordering information is available for your nearest sales organization www.addresses.endress.comor in the Product Configurator under www.endress.com

- 1. Click Corporate
- 2. Select the country
- 3. Click Products
- 4. Select the product using the filters and search field
- 5. Open the product page

The Configuration button to the right of the product image opens the Product Configurator.

#### Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

#### 5-point linearity protocol


#### Conditions for 5-point linearity protocol

- The 5-point linearity protocol applies for the entire measuring system, consisting of the sensor and transmitter. When ordering, specify the transmitter sensor input where the sensor is to be
- The linearization test is conducted under the reference operating conditions of the transmitter.

#### Position of the linearization points

- The 5 points of the linearity protocol are evenly distributed over the span S.
- In order to define the span, values for **Empty calibration** (E) and **Full calibration** (F) must be specified when ordering.
- The specified values are only used to create the linearity protocol. **Empty calibration** and **Full calibration** are then reset to their factory settings.

#### Conditions for defining the span

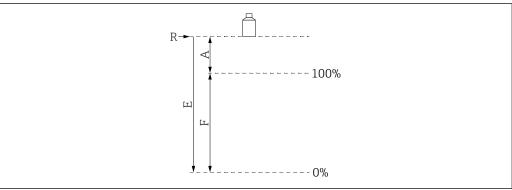

#### ■ 12 Variables to define the span

- Reference point (sensor membrane)
- "Empty calibration" (distance from sensor membrane to 0%-point) F.
- F "Full calibration" (distance from 0%-point to 100%-point)
- Distance from sensor membrane to 100%-point
- $E \le 20000 \text{ mm}$  (787 in)
- F = 200 to 19600 mm (7.87 to 772 in)
- $A \ge 400 \text{ mm} (15.7 \text{ in})$

#### Scope of delivery

- Ordered version of the sensor
- For certified versions: Safety Instructions (XAs)
- For sensors with G1" process connection: counter nut (PA6.6) and seal (EPDM)


#### Accessories

#### Sensor extension cable



- Maximum permissible total length (sensor cable + extension cable): 300 m (984 ft)
   The sensor cable and extension cable are the same type of cable.
- Cable type: LiYCY 2x(0.75)
- Material: PVC
- Ambient temperature: -40 to +105 °C (-40 to +221 °F)
- Order number: 71027742

#### Screw-in flange FAX50

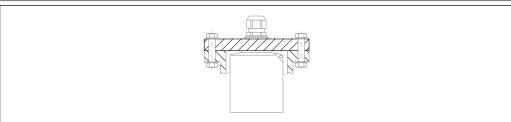




- Mounting on the rear thread G1 or NPT1
- Available flange sizes: see Product Configurator
- Minimum nominal diameter: DN80 / NPS 3"

#### Cantilever arm for the sensors

#### **Application**

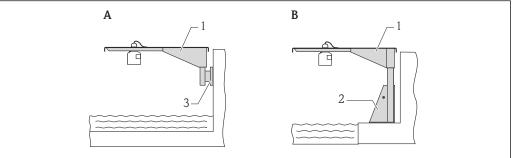

- Mounting of sensor with cantilever arm
- Installation on arm with wall bracket
- Installation on arm with mounting frame
- 1 Cantilever
- 2 Mounting frame
- Wall bracket


#### Use of orifices

- 35 mm (1.4 in) orifice Sensor with counter nut
- 22 mm (0.9 in) orifice

Temperature sensor (e.g. Omnigrad TR61 with TA50 process connection)

#### **Dimensions**

Cantilever arm 500 mm, for G 1" or MNPT 1" connections on rear

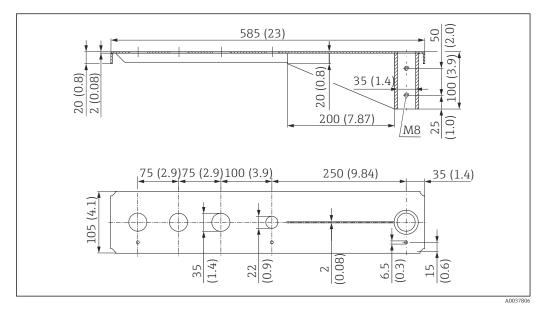

■ 14 Dimensions. Unit of measurement mm (in)

#### Weight:

3.0 kg (6.62 lb)

#### Material


316L (1.4404)

#### Order number

71452315

- i
- 35 mm (1.38 in) openings for all G 1" or MNPT 1" connections on rear
- 22 mm (0.87 in) opening can be used for any additional sensor
- Retaining screws are included in delivery

Cantilever arm 1000 mm, for G 1" or MNPT 1" connections on rear

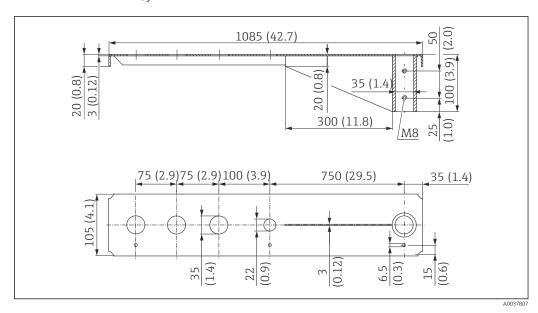

■ 15 Dimensions. Unit of measurement mm (in)

#### Weight:

5.4 kg (11.91 lb)

#### Material

316L (1.4404)


#### Order number

71452316



- $\, \bullet \,$  35 mm (1.38 in) openings for all G 1" or MNPT 1" connections on rear
- 22 mm (0.87 in) opening can be used for any additional sensor
- Retaining screws are included in delivery

#### Frame, 700 mm (27.6 in)

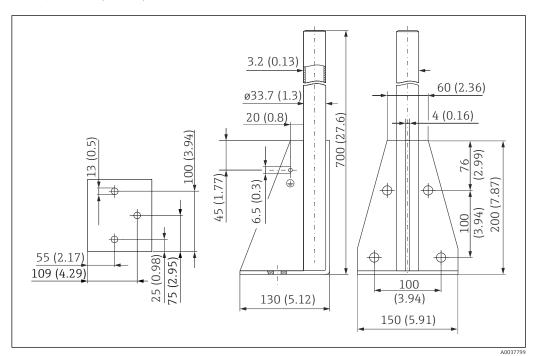

■ 16 Dimensions. Unit of measurement mm (in)

Weight:

4.0 kg (8.82 lb)


Material

316L (1.4404)

Order number

71452327

#### Frame, 1400 mm (55.1 in)

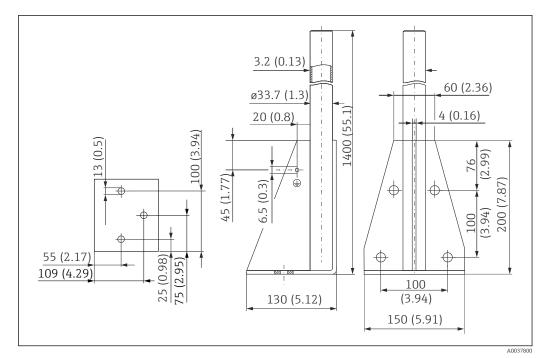

■ 17 Dimensions. Unit of measurement mm (in)

Weight:

6.0 kg (13.23 lb)


Material

316L (1.4404)

Order number

71452326

#### Wall bracket for cantilever with pivot

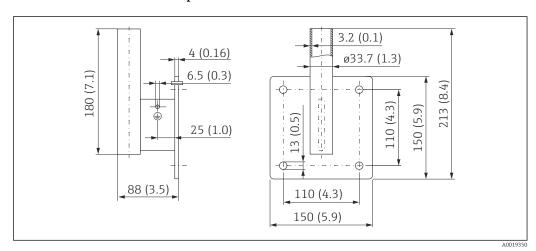

 $\blacksquare$  18 Dimensions of the wall bracket. Unit of measurement mm (in)

Weight

1.21 kg (2.67 lb)

Material


316L (1.4404)

Order number

71452323

18

## Mounting bracket for ceiling mounting

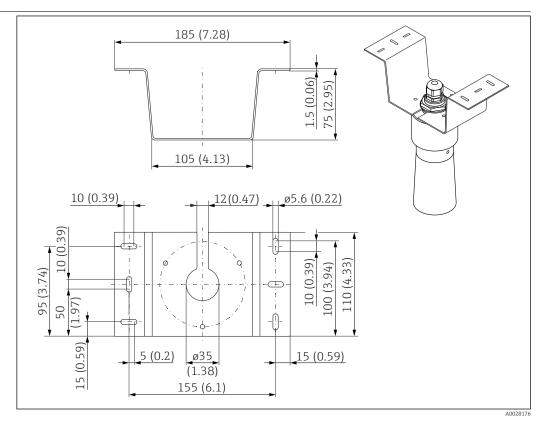

Mounting bracket for ceiling mounting. Unit of measurement mm (in)

Material: 316L (1.4404)Order No.: 71093130

#### FAU40 alignment unit


#### Use

 $\, \blacksquare \,$  To align an ultrasonic sensor with the bulk solids surface

• Swivel range: 15°

Zone separation for explosion hazardous areas

#### **Dimensions**

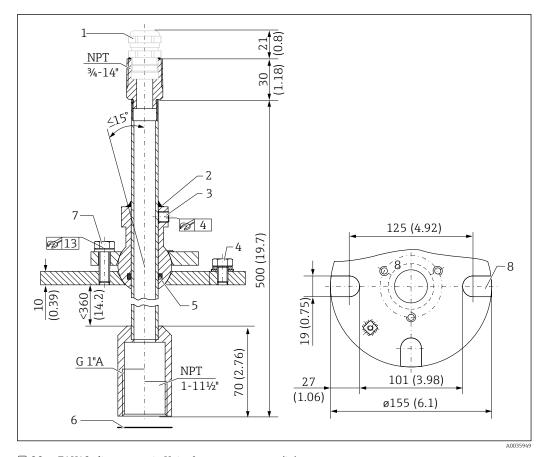

🗷 20 FAU40 alignment unit. Unit of measurement mm (in)

- 1 Cable gland M20x1.5 (if selected in the product structure)
- 2 Seal here
- 3 Two Allen screws for height adjustment (8 Nm (6 lbf ft) $\pm$ 2 Nm ( $\pm$ 1.5 lbf ft))
- 4 Grounding screw
- 5 O-ring
- 6 Seal supplied with the sensor, must be used for applications in ATEX Zone 20
- Screw for lateral adjustment (18 Nm (13.5 lbf ft) $\pm$ 2 Nm ( $\pm$ 1.5 lbf ft))
- 8 Mounting slots (on version with UNI flange)

#### Additional information



Technical Information TI00179F

IP66 protective housing for RNB130 power supply unit

■ **Order number**: 51002468

• Additional information: Technical Information TI00080R

### Supplementary documentation

## Documentation for FMU90 transmitter

- Technical Information TI00397F
- Operating Instructions:
  - BA00288F (HART, level measurement)
  - BA00289F (HART, flow measurement)
  - BA00292F (Profibus DP, level measurement)
  - BA00293F (Profibus DP, flow measurement)
- Description of Device Parameters: GP01151F

### Documentation for FMU95 transmitter

- Technical Information TI00398F
- Operating Instructions: BA00344F
- Description of Device Parameters: GP01152F

#### Other documentation



Further information and the documentation currently available can be found on the Endress+Hauser- website: www.endress.com  $\rightarrow$  Downloads.





www.addresses.endress.com