

# Technical Information

## Liquiphant Density and Density Computer FML621

Vibronic



Density computer for liquids  
Also for use in hazardous areas

### Application

The density measuring line can be used in liquid media. It is used for the following purposes:

- To density measurement
- To intelligent medium detection
- To calculate the reference density
- To calculate the concentration of a liquid
- To convert values to different units such as °Brix, °Baumé, °API etc.

### Your benefits

- Measurement used directly in tanks or pipes without the need for additional pipework
- Integration of existing temperature measurements for temperature compensation
- Additional calculations, such as the concentration of a product, can be performed in the Density Computer FML621

## Table of contents

<b>Important document information</b> . . . . .	<b>3</b>	<b>FML621 installation instructions</b> . . . . .	<b>28</b>
Notes on safety conventions and icons . . . . .	3	Mounting location . . . . .	28
<b>Application</b> . . . . .	<b>4</b>	Orientation . . . . .	28
Density measurement . . . . .	4	<b>Environment</b> . . . . .	<b>28</b>
<b>Function and system design</b> . . . . .	<b>6</b>	Ambient temperature range . . . . .	28
Measuring principle . . . . .	6	Storage temperature . . . . .	28
System design . . . . .	6	Climate class . . . . .	28
Specific density applications . . . . .	7	Electrical safety . . . . .	28
Measuring system . . . . .	8	Degree of protection . . . . .	28
Modularity . . . . .	8	Electromagnetic compatibility . . . . .	28
Design . . . . .	8	<b>Installation conditions for Liquiphant</b> . . . . .	<b>29</b>
Electronic insert for density measurement . . . . .	9	Orientation . . . . .	29
<b>Input</b> . . . . .	<b>9</b>	Inlet and outlet run . . . . .	29
Measured variable . . . . .	9	Mounting location and correction factor . . . . .	30
Input signal . . . . .	9	<b>Ambient conditions for Liquiphant Density</b> . . . . .	<b>33</b>
Measuring range . . . . .	9	Ambient temperature range . . . . .	33
Galvanic isolation . . . . .	11	<b>Mechanical construction</b> . . . . .	<b>33</b>
<b>Output</b> . . . . .	<b>11</b>	Terminals . . . . .	33
Output . . . . .	11	Design . . . . .	33
Switching output . . . . .	12	<b>Display and operating elements</b> . . . . .	<b>34</b>
Transmitter power supply and an external power supply . . . . .	12	Display elements . . . . .	34
<b>Electrical connection</b> . . . . .	<b>12</b>	Operating elements . . . . .	35
Slots and block circuit diagram . . . . .	12	Remote operation . . . . .	35
Terminal assignment . . . . .	14	Real time clock . . . . .	35
Connecting the power supply . . . . .	15	<b>Certificates and approvals</b> . . . . .	<b>36</b>
Connecting density sensor . . . . .	16	CE mark . . . . .	36
E+H - specific devices . . . . .	17	Ex approval . . . . .	36
Connecting outputs . . . . .	18	Other standards and guidelines . . . . .	36
Interface connection . . . . .	19	<b>Ordering information</b> . . . . .	<b>36</b>
Ethernet option . . . . .	19	<b>Accessories</b> . . . . .	<b>36</b>
The extension cards . . . . .	20	General . . . . .	36
Connecting remote display unit and the operating unit . . . . .	25	Extension cards . . . . .	37
Post-connection check . . . . .	26	<b>Documentation</b> . . . . .	<b>37</b>
<b>Power supply</b> . . . . .	<b>26</b>	Brief Operating Instructions (KA) . . . . .	37
Supply voltage . . . . .	26	Operating Instructions (BA) . . . . .	37
Power consumption . . . . .	26	Safety Instructions (XA) . . . . .	37
Connection data interface . . . . .	26		
<b>Reference operating conditions</b> . . . . .	<b>27</b>		
FML621 reference operating conditions . . . . .	27		
Reference operating conditions for special calibration and Liquiphant M Density . . . . .	27		
<b>Performance characteristics</b> . . . . .	<b>27</b>		
General measuring conditions for accuracy data . . . . .	27		
Maximum measured error . . . . .	27		
Non-repeatability - reproducibility . . . . .	27		
Factors influencing accuracy data . . . . .	28		

## Important document information

### Notes on safety conventions and icons

#### Safety symbols

##### **DANGER**

This symbol alerts you to a dangerous situation. Failure to avoid this situation will result in serious or fatal injury.

##### **WARNING**

This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in serious or fatal injury.






##### **CAUTION**

This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.




##### **NOTICE**

This symbol contains information on procedures and other facts which do not result in personal injury.



#### Electrical symbols

Symbol	Meaning
	Direct current
	Alternating current
	Direct current and alternating current
	<b>Ground connection</b> A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	<b>Protective Earth (PE)</b> A terminal which must be connected to ground prior to establishing any other connections.  The ground terminals are situated inside and outside the device: <ul style="list-style-type: none"> <li>■ Inner ground terminal: Connects the protective earth to the mains supply.</li> <li>■ Outer ground terminal: Connects the device to the plant grounding system.</li> </ul>

#### Symbols for certain types of information

Symbol	Meaning
1, 2, 3 ...	Item numbers
	Series of steps
A, B, C, ...	Views
A-A, B-B, C-C, ...	Sections
	<b>Hazardous area</b> Indicates a hazardous area.
	<b>Safe area (non-hazardous area)</b> Indicates the non-hazardous area.


#### Symbols at the device

Symbol	Meaning
	<b>Safety instructions</b> Observe the safety instructions contained in the associated Operating Instructions.
	<b>Temperature resistance of the connection cables</b> Specifies the minimum value of the temperature resistance of the connection cables.

## Application

### Density measurement

The Liquiphant FTL51B with electronic insert FEL60D measures the density of a liquid medium in pipes and tanks. The device is suitable for all Newtonian - ideal viscous - fluids. The device is also suitable for use in hazardous areas.

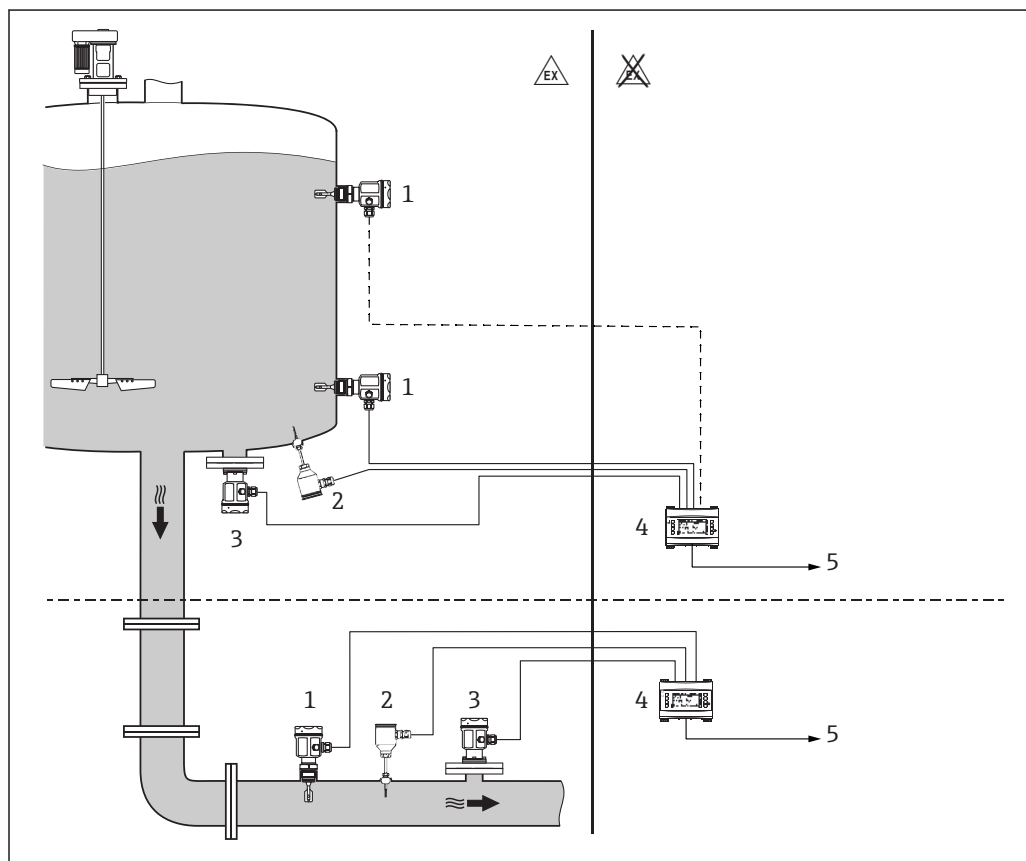

A0039632

#### 1 Density measurement with FML621

- 1 Liquiphant FTL51B sensor with electronic insert FEL60D - pulse output
- 2 Temperature sensor - e.g. 4 to 20 mA output
- 3 Pressure transmitter 4 to 20 mA output required for pressure changes >6 bar
- 4 Liquiphant Density Computer FML621 with display and operating unit
- 5 PLC



The measurement can be affected by:

- air bubbles at the sensor
- unit not fully covered by the medium
- solid media buildup on the sensor
- high fluid velocity in pipes
- severe turbulence in the pipe due to inlet and outlet runs that are too short (→ 29)
- corrosion of the fork
- non-Newtonian - non-ideal viscous - behavior of the fluids

### Application examples: basic unit

#### *1 density measuring line pressure and temperature-compensated*

- **Product structure:** FML621-xxxAAxxxx
- **Number of inputs:** 4x pulse input for 0 to 20 mA or 4 to 20 mA
- **Number of outputs:** 1x relay SPST, 2x 0 to 20 mA or 4 to 20 mA
- **Comment:**
  - 1 Liquiphant with FEL60D
  - 1 temperature transmitter 4 to 20 mA
  - 1 pressure transmitter 4 to 20 mA
  - 1 output: density 4 to 20 mA
  - 1 output: temperature 4 to 20 mA

#### *2 density measuring lines temperature-compensated*

- **Product structure:** FML621-xxxAAxxxx
- **Number of inputs:** 4x pulse input for 0 to 20 mA or 4 to 20 mA
- **Number of outputs:** 1x relay SPST, 2x 0 to 20 mA or 4 to 20 mA
- **Comment:**
  - 2 Liquiphant with FEL60D
  - 2 temperature transmitter 4 to 20 mA
  - 1 output: density 4 to 20 mA
  - 1 output: temperature 4 to 20 mA

### Application examples: Basic unit + 2 extension cards

#### *3 density measuring lines, 2x temperature-compensated, 1x pressure, and temperature compensated*

- **Product structure:** FML621-xxxBBxxxx
- **Number of inputs:** 8x pulse input for 0 to 20 mA or 4 to 20 mA
- **Number of outputs:** 5x relay SPST, 6x 0 to 20 mA or 4 to 20 mA
- **Comment:**
  - 3 Liquiphant with FEL60D
  - 3 temperature transmitter 4 to 20 mA
  - 1 pressure transmitter 4 to 20 mA
  - 3 outputs: density 4 to 20 mA
  - 3 outputs: temperature 4 to 20 mA
  - 1 relay for medium detection

### Application examples: medium detection

#### *Distinguish between 2 media*

- **Product structure:** FML621-xxxAAxxxx Basic unit
- **Use of inputs:**
  - 1x FEL60D
  - 1x temperature 4 to 20 mA
- **Information content:**
  - 1 output: density 4 to 20 mA
  - 1 output: temperature 4 to 20 mA
  - 1 relay
- **Comment:** The medium detection can refer to concentrations or phase transitions

#### *Distinguish between 3 media*

- **Product structure:** FML621-xxxBAxxxx Basic unit with additional relay card
- **Use of inputs:**
  - 1x FEL60D
  - 1x temperature 4 to 20 mA
- **Information content:**
  - 1 output: density 4 to 20 mA
  - 1 output: temperature 4 to 20 mA
  - 1 relay: display product 1
  - 1 relay: display product 2
  - 1 relay: display product 3
- **Comment:** The relays can activate subsequent processes by triggering actuators

### Application examples: density

#### Density measurement or concentration calculation with pump protection


- **Product structure:** FML621-xxxBAxxxx Basic unit
- **Use of inputs:**
  - 1x FEL60D
  - 1x temperature 4 to 20 mA
- **Information content:**
  - 1 output: density 4 to 20 mA
  - 1 output: temperature 4 to 20 mA
  - 1 relay to switch off the pump
- **Comment:** In addition to determine the density and the concentration, a pump protection can also be implemented by setting the appropriate switching frequency.

## Function and system design

### Measuring principle

A piezoelectric drive excites the tuning fork of the Liquiphant Density to its resonance frequency. If the density of the liquid medium changes, then the resonance frequency of the tuning fork also changes. The density of the medium has a direct impact on the resonance frequency of the tuning fork. By storing specific medium properties and mathematic relations in the system, the exact concentration of the medium can be calculated.

### System design

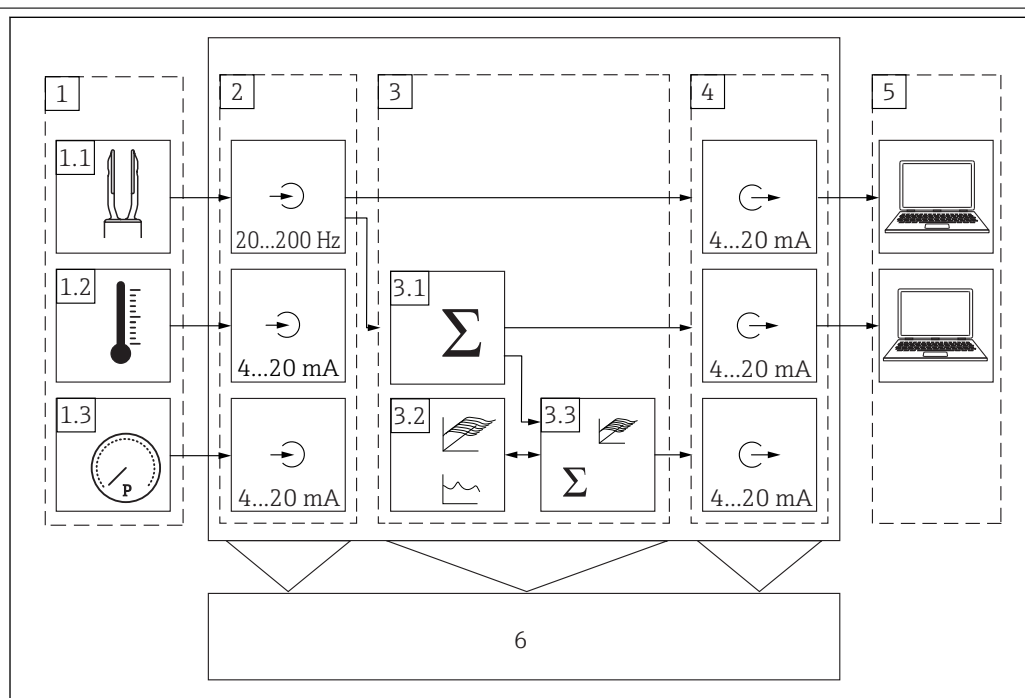

A0039647

2 FML621 modular schema

- 1 External sensors
- 1.1 Liquiphant Density FTL51B
- 1.2 Temperature sensor
- 1.3 Pressure sensor
- 2 Input modules
- 3 Calculation module
- 3.1 Maths e.g. density
- 3.2 2D/3D curve
- 3.3 Maths e.g. concentration, 3D linearization
- 4 Output modules
- 5 Information processing - control room
- 6 Display

## Specific density applications

Available software modules calculate the density from the frequency, temperature and pressure input variables.


### Operating principle

The vibrating frequency of the tuning fork is reduced when the fork is completely covered with liquid. The corresponding density of the medium can be calculated using other information, such as the temperature and pressure. If the value by which the density has changed is known, the concentration of the medium can be determined using a function stored in the system. This value can be determined empirically or be based on existing tables. The tables for converting density to concentration must be provided by the customer.

Additional software modules can calculate the density at the reference temperature, compute the concentrations or detect media.

### Reference density

In this module, the system refers back to a reference temperature, such as 15 °C (59 °F) or 20 °C (68 °F). It must be known how the density of the medium changes at different temperatures.

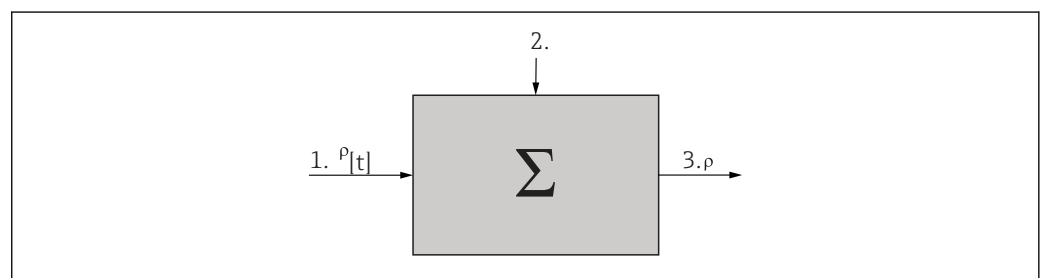


A0039650

- 1 Input data: Table  $\rho$  [t]
- 2 Measured liquid medium: temperature and density
- 3 Output: Calculated density  $\rho$  [standard]

### Concentration

Using density and concentration curves already available or determined empirically, the concentration can be determined when substances are continuously dissolved in a medium.

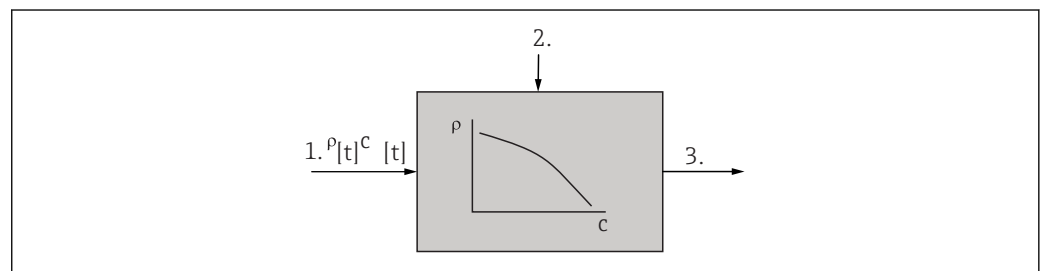


A0039651

- 1 Input data: Table  $\rho, c$  [t]
- 2 Measured liquid medium: temperature and density
- 3 Output: Calculated concentration

### Medium detection

To be able to distinguish between two media, the density function - as a function of the temperature - can be stored for several media. In this way, the system can distinguish between two media.

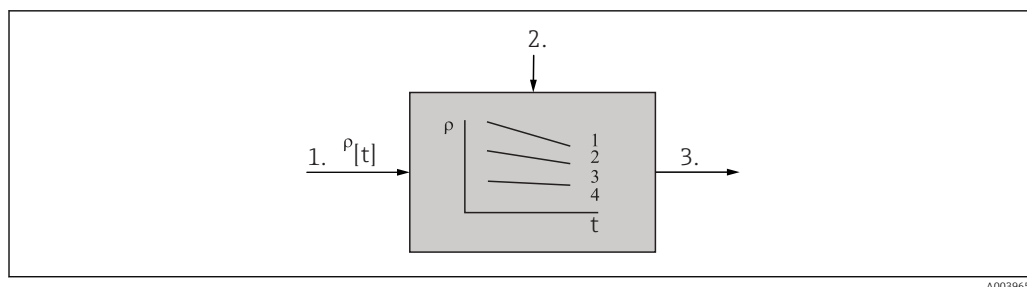

A0039652


- 1 Input data: Tables  $\rho[t]$  for two liquid mediums
- 2 Measured liquid medium: temperature and density
- 3 Output: Analog output device

## Measuring system

The FML621 supplies power directly to two-wire transmitters which are connected. Intrinsically safe inputs and transmitter power supply units for current cards are optionally available for hazardous applications. The inputs, outputs, limit values and display are configured, and the device is commissioned and serviced, via 8 soft keys, with the backlit dot-matrix display, using an RS232 or RS485 interface or PC software ReadWin® 2000. The device can be extended using additional extension cards.

The change of the background color signals the alarms or violations of the values. The background color is configurable.

To use the telealarm function, we recommend common industrial modems that have an RS232 interface. The measured values and events or alarms are coded in accordance with the serial protocol and transmitted. The type of the protocol can be requested.

 The number of inputs, outputs, relays, and transmitter power supply units contained in the basic unit can be individually extended using a maximum of three plug-in cards.

## Modularity



Measuring the density of a liquid medium. Liquiphant with electronic insert FEL60D and Density Computer FML621. Also for hazardous areas. Up to five density measuring lines can be operated using Density Computer FML621. All slots must be fitted with plug-in cards.

The Liquiphant set measures density of a liquid medium also in hazardous area. The Density Computer FML621 operates up to 5 measuring lines. All slots must be fitted with plug-in cards.

### Density Computer FML621 specification

- **Input**
  - FEL60D sensor
  - 0 to 20 mA or 4 to 20 mA pulse inputs
  - 0 to 18 digital inputs
  - 4 to 10 relays inputs
  - sensors (mA, mV, V, TC, RTD)
- **Output**
  - 2 to 8 analog outputs 0 to 20 mA or 4 to 20 mA
  - 2 to 8 pulse outputs - active or passive
  - 1 to 19 relays SPST, AC or DC
- **Communication**
  - Ethernet IP
  - PSTN or GSM modem
  - Serial bus RS232, RS485
  - ProfiBus® via coupler
  - ReadWin® 2000 PC software
- **Power supply mode**
  - 4-10 devices, max. current consumption 30 mA
  - 1 device, max. current consumption 80 mA
- **Internal memory**
  - 512 kB
- **Calculating functions**
  - predefined
  - editable

## Design

 Information on the mechanical construction of Liquiphant M sensors is provided in the Technical Information. The document numbers for downloading the documents on the Internet [www.endress.com](http://www.endress.com) are listed on →  37.



### Density Computer FML621

#### Liquiphant Density FTL51B

Compact version or with extension pipe and with AlloyC22 for use in aggressive liquids

#### Electronic insert for density measurement

Liquiphant Density with electronic insert FEL60D.

For Density Computer FML621, two-wire pulse output.

Current pulses superimposed on the power supply along the two-wire cabling.

## Input

#### Measured variable

##### Input: voltage

- analog
- digital

##### Input: current

- analog
- PFM
- pulse



Only Endress+Hauser flow sensors can be connected to the PFM input.

Not suitable for level and pressure measuring instruments.

#### Input signal

Any measured variable like flow, level, pressure, temperature or density is implemented as an analog signal.

#### Measuring range

##### Current

- 0 to 20 mA or 4 to 20 mA +10 % overrange
- max. input current: 150 mA
- input impedance: <10 Ω
- accuracy 0.1 % of full scale value
- temperature drift: 0.04 % / K (0.022 % / °F)
- signal damping low filter 1st order, filter constant adjustable 0 to 99 s
- resolution: 13 bit

##### Current (U-I-TC card)

- 0 to 20 mA or 4 to 20 mA +10 % overrange
- max. input current: 80 mA
- input impedance: =10 Ω
- accuracy: 0.1 % of full scale value
- temperature drift: 0.01 % / K 0.01 % / K (0.0056 % / °F)

##### PFM/pulse input

- frequency range: 0.01 to 18 kHz
- signal level - with approx.: 1.3 kΩ dropping resistor at max. 24 V voltage level:
  - low: 2 to 7 mA
  - high: 13 to 19 mA
- measurement method: period length or frequency measurement
- temperature drift: 0.01 % over entire temperature range

##### Voltage (digital input)

- voltage level:
  - low: -3 to 5 V
  - high: 12 to 30 V (as per IEC 61131-2)
- input current typically: 3 mA with overload and reverse polarity protection
- sampling frequency:
  - 4x 4 Hz
  - 2x 20 kHz or 2x 4 Hz

##### Voltage (analog input)

- voltage: 0 to 10 V<sub>rms</sub>, 0 to 5 V, ±10 V, inaccuracy ±0.1 % of measuring range, input impedance >400 kΩ
- voltage: 0 to 100 mV, 0 to 1 V, ±1 V, ±100 mV, measured error ±0.1 % of measuring range, input impedance >1 MΩ
- temperature drift: 0.01 % / K (0.0056 % / °F)

#### Resistance thermometer Pt100 as per ITS 90

- measuring range: -200 to 800 °C (-328 to 1472 °F)
- accuracy: - 4-wire connection 0.03 % of full scale value
- type of connection: 3-wire or 4-wire system
- measuring current: 500 µA
- resolution: 16 bit
- temperature drift: 0.01 % / K (0.0056 % / °F)

#### Resistance thermometer Pt500 as per ITS 90

- measuring range: -200 to 250 °C (-328 to 482 °F)
- accuracy: - 4-wire connection 0.1 % of full scale value
- type of connection: 3-wire or 4-wire system
- measuring current: 500 µA
- resolution: 16 bit
- temperature drift: 0.01 % / K (0.0056 % / °F)

#### Resistance thermometer Pt1000 as per ITS 90

- measuring range: -200 to 250 °C (-328 to 482 °F)
- accuracy: - 4-wire connection 0.08 % of full scale value
- type of connection: 3-wire or 4-wire system
- measuring current: 500 µA
- resolution: 16 bit
- temperature drift: 0.01 % / K (0.0056 % / °F)

#### Thermocouples (TC)

- J (Fe-CuNi), IEC 584
  - measuring range: -210 to 999.9 °C (-346 to 1832 °F)
  - accuracy: ± (0.15 % oMR + 0.5 K) as of -100 °C  
± (0.15 % oMR + 0.9 °F) as of -148 °F
- K (NiCr-Ni), IEC 584
  - measuring range: -200 to 1372 °C (-328 to 2502 °F)
  - accuracy: ± (0.15 % oMR + 0.5 K) as of -130 °C  
± (0.15 % oMR + 0.9 °F) as of -202 °F
- T (Cu-CuNi), IEC 584
  - measuring range: -270 to 400 °C (-454 to 752 °F)
  - accuracy: ± (0.15 % oMR + 0.5 K) as of -200 °C  
± (0.15 % oMR + 0.9 °F) as of -382 °F
- N (NiCrSi-NiSi), IEC 584
  - measuring range: -270 to 1300 °C (-454 to 1386 °F)
  - accuracy: ± (0.15 % oMR + 0.5 K) as of -100 °C  
± (0.15 % oMR + 0.9 °F) as of -148 °F
- B (Pt30Rh-Pt6Rh), IEC 584
  - measuring range: 0 to 1820 °C (32 to 3308 °F)
  - accuracy: ± (0.15 % oMR + 1.5 K) as of 600 °C  
± (0.15 % oMR + 2.7 °F) as of 1112 °F
- D (W3Re/W25Re), ASTM E 998
  - measuring range: 0 to 2315 °C (32 to 4199 °F)
  - accuracy: ± (0.15 % oMR + 1.5 K) as of 500 °C  
± (0.15 % oMR + 2.7 °F) as of 932 °F
- C (W5Re/W26Re), ASTM E 998
  - measuring range: 0 to 2315 °C (32 to 4199 °F)
  - accuracy: ± (0.15 % oMR + 1.5 K) as of 500 °C  
± (0.15 % oMR + 2.7 °F) as of 932 °F
- L (Fe-CuNi), DIN 43710, GOST
  - measuring range: -200 to 900 °C (-346 to 1652 °F)
  - accuracy: ± (0.15 % oMR + 0.5 K) as of -100 °C  
± (0.15 % oMR + 0.9 °F) as of -148 °F

- U (Cu-CuNi), DIN 43710
  - measuring range: -200 to 900 °C (-346 to 1 652 °F)
  - accuracy:  $\pm (0.15 \% \text{ oMR} + 0.5 \text{ K})$  as of -100 °C  
 $\pm (0.15 \% \text{ oMR} + 0.9 \text{ °F})$  as of -148 °F
- S (Pt10Rh-Pt), IEC 584
  - measuring range: 0 to 1 768 °C (32 to 3 214 °F)
  - accuracy:  $\pm (0.15 \% \text{ oMR} + 3.5 \text{ K})$  for 0 to 100 °C  
 $\pm (0.15 \% \text{ oMR} + 1.5 \text{ K})$  as of 100 to 1 768 °C  
 $\pm (0.15 \% \text{ oMR} + 6.3 \text{ °F})$  for 0 to 212 °F  
 $\pm (0.15 \% \text{ oMR} + 2.7 \text{ °F})$  for 212 to 2 314 °F
- R (Pt13Rh-Pt), IEC 584
  - measuring range: 0 to 1 768 °C (32 to 3 214 °F)
  - accuracy:  $\pm (0.15 \% \text{ oMR} + 3.5 \text{ K})$  for 0 to 100 °C  
 $\pm (0.15 \% \text{ oMR} + 1.5 \text{ K})$  as of 100 to 1 768 °C  
 $\pm (0.15 \% \text{ oMR} + 6.3 \text{ °F})$  for 0 to 212 °F  
 $\pm (0.15 \% \text{ oMR} + 2.7 \text{ °F})$  for 212 to 2 314 °F

#### Galvanic isolation

The inputs are galvanically isolated between the individual extension cards and the basic unit (→ 11).



With digital inputs, every terminal block is galvanically isolated from each other.

## Output

#### Output

##### Output signal

Current, pulse, transmitter power supply (MUS) and switching output.

##### Galvanic isolation

- the signal inputs and outputs are galvanically isolated towards the supply voltage  
testing voltage: 2.3 kV
- all the signal inputs and outputs are galvanically isolated from one another  
testing voltage: 500 V



The specified isolation voltage is the AC testing voltage  $U_{\text{eff}}$ , which is applied between the connections. Basis for assessment: IEC 61010-1, protection class II, overvoltage category II.

##### Measured variables

##### Current

- 0 to 20 mA or 4 to 20 mA +10 % overrange, invertible
- max. loop current: 22 mA - short-circuit current
- load max.: 750  $\Omega$  at 20 mA
- accuracy: 0.1 % of full scale value
- temperature drift: 0.1 % / 10 K (0.056 % / 10 °F) ambient temperature
- output ripple: <10 mV at 500  $\Omega$  for frequencies <50 kHz
- resolution: 13 bit
- error signals: 3.6 mA or 21 mA limit as per NAMUR NE 43 - adjustable

##### Pulse

- basic unit:
  - frequency range: up to 12.5 kHz
  - voltage level: 0 to 1 V low, 12 to 28 V high
  - load min.: 1 k $\Omega$
  - pulse width: 0.04 to 1 000 ms
- extension cards - digital passive, open collector:
  - frequency range: up to 12.5 kHz
  - $I_{\text{max}} = 200 \text{ mA}$
  - $U_{\text{max}} = 24 \text{ V} \pm 15 \%$
  - $U_{\text{low/max}} = 1.3 \text{ V}$  at 200 mA
  - pulse width: 0.04 to 1 000 ms

### Number

- number:
  - 2x 0 to 20 mA or 4 to 20 mA / pulse - in basic unit
  - ethernet option: no current output present in the basic unit
- max. number:
  - 8x 0 to 20 mA or 4 to 20 mA / pulse - depends on the number of extension cards
  - 6x digital passive - depends on the number of extension cards

### Signal sources

all available multifunctional inputs and results from mathematic calculations can be freely allocated to the outputs.

## Switching output

### Function

Limit relay switches in the operating modes: minimum or maximum safety, gradient, alarm, frequency or pulse, device error.

### Switch behavior

Binary, switches when the limit value is reached - potential-free NO contact.

### Relay switching capacity

Max. 250 V<sub>AC</sub> 3 A / 30 V<sub>DC</sub> 3 A



Do not combine line voltage and protective extra low voltage for extension card relays.

### Switching frequency

Maximum 5 Hz

### Threshold

Freely programmable

### Hysteresis

0 to 99 %

### Signal source

All available inputs and calculated variables can be allocated freely to the switching outputs.

### Number of switching cycles

> 100,000

### Scan rate

500 ms

### Number

- 1 relay - in the basic unit
- Maximum number: 19 relays - depend on the number and type of extension cards

## Transmitter power supply and an external power supply

### The transmitter power supply unit (MUS), terminals 81/82 or 81/83 - the optional power extension cards 181/182 or 181/183

- maximum output voltage: 24 V<sub>DC</sub> ±15 %
- impedance: <345 Ω
- maximum loop current: 22 mA (at U<sub>out</sub> >16 V)

### FML621 technical data:

- HART® communication is not impaired
- number: 4 MUS in the basic unit
- maximum number: 10 - depends on the number and type of extension cards

### Additional power supply terminals 91/92:

- supply voltage: 24 V<sub>DC</sub> ±5 %
- current max.: 80 mA, short-circuit proof
- number: 1
- source resistance: <10 Ω


## Electrical connection

### Slots and block circuit diagram



### Destruction of electronic components.

- ▶ Do not install or wire the device when it is connected to the power supply.

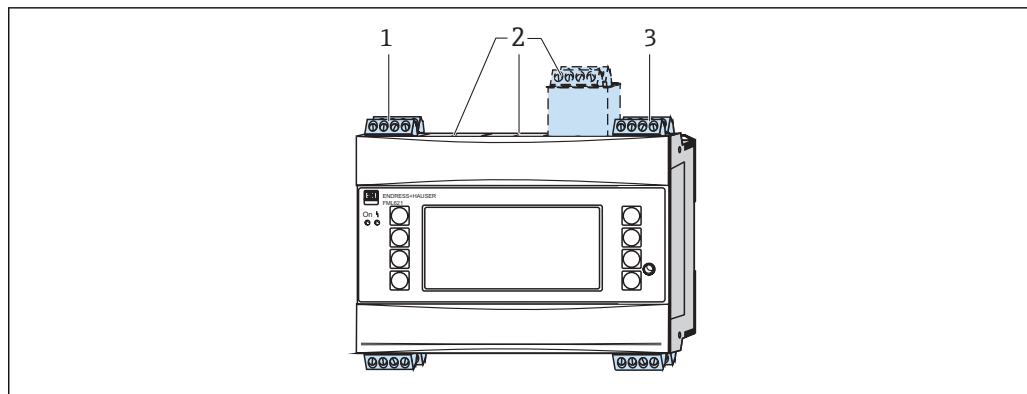

A0039653

3 Base unit with extension cards.

1 Slot with extension card A

2 Slots B, C, D


3 Slot with extension card E

### Slots specification

- Slot A
  - input: 2x density sensors, 0 to 20 mA or 4 to 20 mA
  - output: 2x 0 to 20 mA or 4 to 20 mA
- Slots B, C, D
  - input: max. 10 analog devices or 18 digital devices
  - output: max. 8 analog devices or 6 digital devices or 19 relays SPST
- Slot E
  - input: 2x density sensors, 0 to 20 mA or 4 to 20 mA
  - output: relay SPST

**i** The extension cards mounted in the A and E slots are integral parts of the basic unit.  
The slots B, C and D can be expanded with additional extension cards.


## Terminal assignment

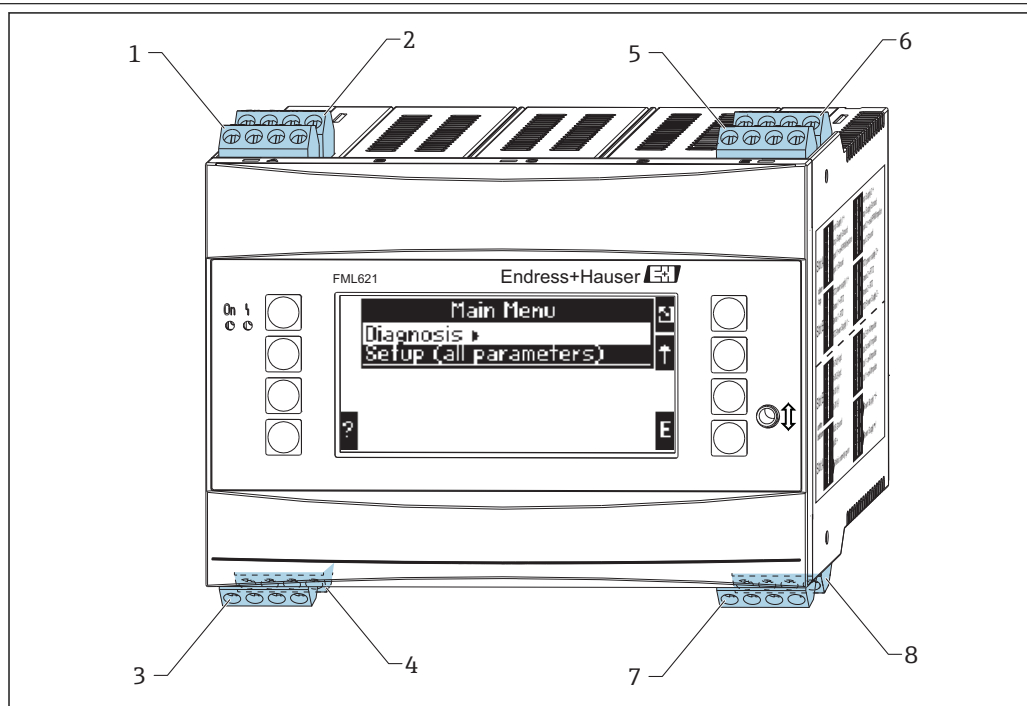

A0039654

## 4 Slot assignment

- 1 Slot A I - input
- 2 Slot A II - input
- 3 Slot A III - output
- 4 Slot A IV - output
- 5 Slot E I - input
- 6 Slot E II - input
- 7 Slot E III - output
- 8 Slot E IV - output

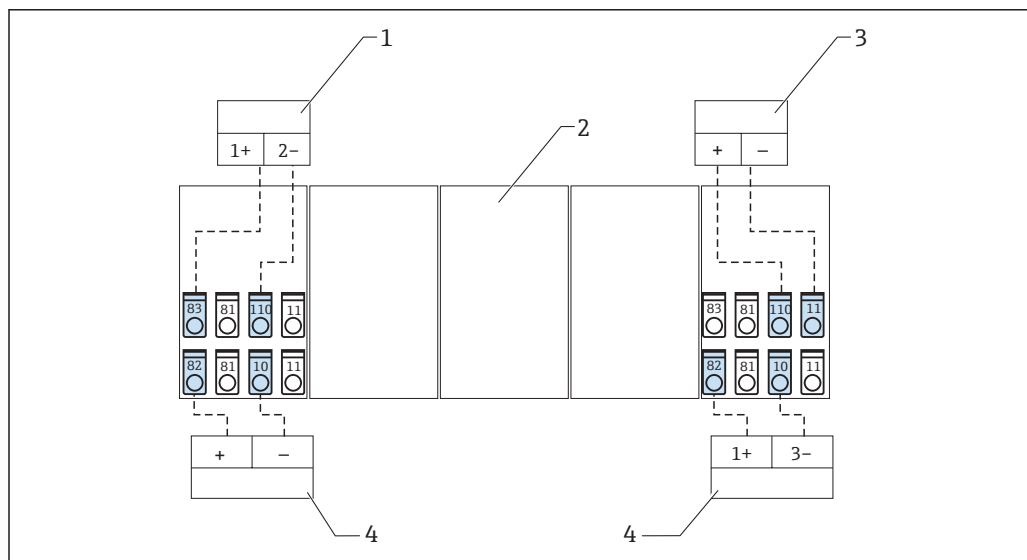


A0039655

## 5 Connection overview - inputs

- 1 Passive sensor - pressure measuring
- 2 Slot for the additional extension card
- 3 Active sensor
- 4 Passive sensor

**i** Active sensor: passing on temperature information from a PLC can be taken as an example for connecting an active sensor.

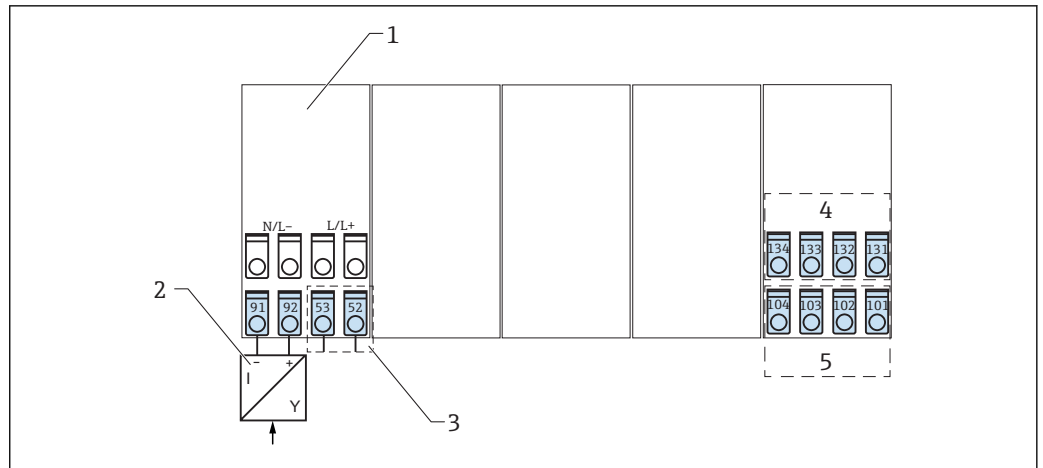

A0039656

6 Connection overview - outputs

- 1 Extension card
- 2 Power supply for sensors
- 3 Relay contact
- 4 Pulse and current outputs - active
- 5 Bus interfaces

**i** With the Ethernet option, the current output or pulse output is not available at slot E.

#### Slot A I

Input: current or PFM or pulse input 1

- terminal 10: 0 to 20 mA or 4 to 20 mA, PFM, pulse input 1
- terminal 11: ground for 0 to 20 mA or 4 to 20 mA, PFM, pulse input
- terminal 81: sensor power supply ground 1
- terminal 82: 24 V sensor power supply 1

#### Slot A II

Input: current or PFM or pulse input 2

- terminal 110: 0 to 20 mA or 4 to 20 mA, PFM, pulse input 2
- terminal 11: ground for 0 to 20 mA or 4 to 20 mA, PFM, pulse input
- terminal 81: sensor power supply ground 2
- terminal 83: 24 V sensor power supply 2

#### Slot A III

Output: relay or additional sensor power supply

- terminal 52: relay Common (COM)
- terminal 53: relay Normally Open (NO)
- terminal 91: sensor power supply ground
- terminal 93: +24 V sensor power supply

#### Slot A IV

Output: power supply

- terminal L/L+: **L** for AC, **L+** for DC
- terminal N/L-: **N** for AC, **L-** for DC

**i** The inputs in the same slot are not galvanically isolated. There is a separation voltage of 500 V between the inputs and outputs in various slots. Terminals with the same second digit are jumpered internally, e.g. the terminals 11 and 81.

#### Connecting the power supply



**WARNING**

Destruction of electronic components.

- Check the power supply voltage is the same as indicated on the label plate of the device.



**DANGER**


High risk of body injuries and damage of the electronic components by the invalid supply voltage.

- For the version of the device, supplied 90 to 250 V voltage, install a switch marked as a separator in the power supply circuit of the device in an easily accessible location.

**⚠ WARNING**
**Lack of protection of the device's power supply circuit.**

Destruction of electronic components.

- Protect the power supply circuit with a 10 A fuse when the device is supplied with 90 to 250 V.

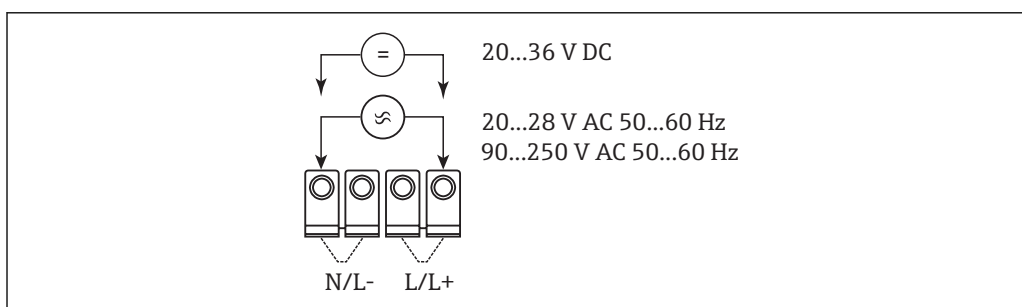

A0039657

7 Power supply connection

## Connecting density sensor


**Liquiphant Density with electronic insert FEL60D**
**⚠ CAUTION**
**Operation with other switching units is not permitted.**

Destruction of electronic components.

- FEL60D cannot be installed in devices that were originally used as a point level switch.

**Two-wire connection at Density Computer FML621**

The output signal is based on pulse technology. With the aid of this signal, the fork frequency is constantly forwarded to the switching unit.

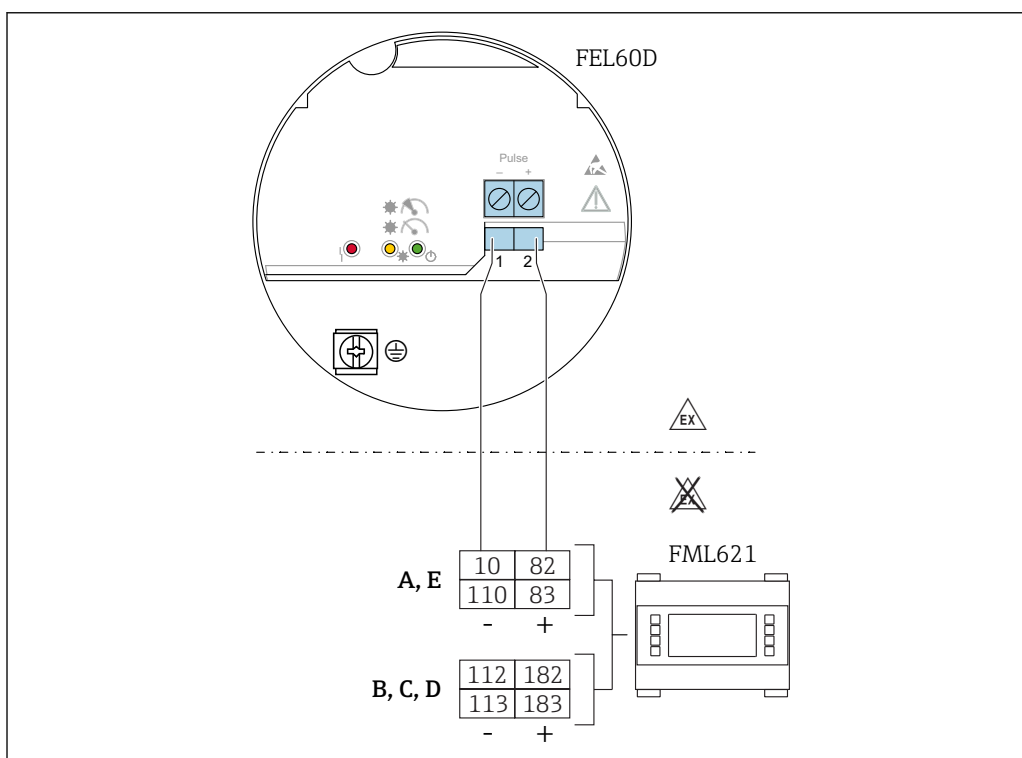

A0036059

8 Connection schema the FEL60D module to Density Computer FML621

**Pulse signal on alarm**

Output signal on power failure or in the event of damaged sensor: 0 Hz.



### Calibration and adjustment

In the Liquiphant modular system, the option of an extended calibration is also provided in addition to the electronics on special calibration, density H<sub>2</sub>O (→ 36).

The three types of adjustment are implemented:

#### Standard adjustment - see: TI01403F, ordering information for additional fittings, basic version A

Two fork parameters are determined at the factory to describe the sensor characteristics and are provided in the adjustment report with the product. These parameters must be transmitted to the Density Computer FML621.

#### Special adjustment - see: TI01403F, ordering information for additional fittings, special adjustment, density H<sub>2</sub>O (K) or special adjustment, density H<sub>2</sub>O with 3.1 certificate (L)

Three fork parameters are determined at the factory to describe the sensor characteristics and are provided in the adjustment report with the product. These parameters must be transmitted to the Density Computer FML621.

This type of adjustment achieves an even greater level of accuracy (→ 27).

#### Field adjustment

During field adjustment, the density value determined by the customer is used for wet adjustment .

**i** More information on Liquiphant is provided in the following "Technical Information" document:  
Liquiphant FTL60D - for standard applications: TI01403F

**i** All of the required parameters of the Liquiphant Density are documented in **Adjustment report** and **Sensor adjustments**.

The documents are included in the delivery.


### E+H - specific devices

**i** The basic version of **Density Computer FML621** is fitted with slots **A** and **E**.

The device can be extended to the slots B, C and D.

**i** The maximum cable length is 1 000 m (3 280.8 ft). The cable must be shielded for EMC requirements. The maximum power supply per core is 25 W.

### Density sensor with a pulse output

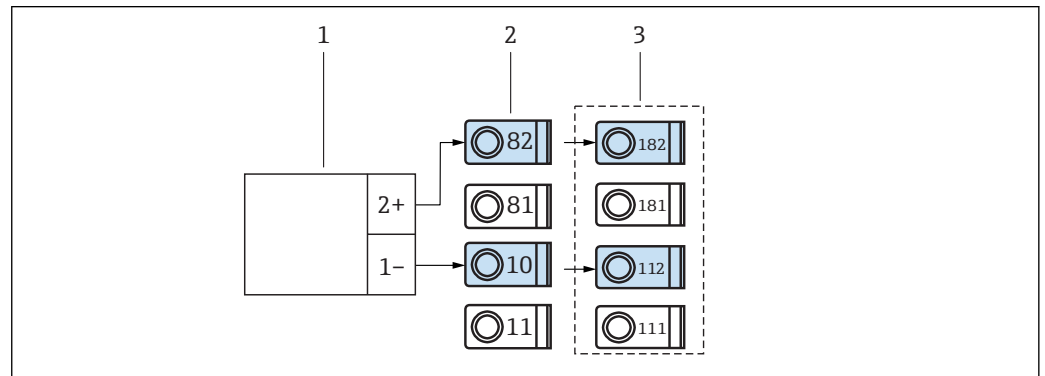


9 Connection of the density sensor with a pulse output

- 1 Density sensor
- 2 Slot A I
- 3 Additional Slot B I

### Temperature sensor via temperature head transmitter

**i** Connection of PT100, PT500 and PT1000 sensors is possible only via an extension card.

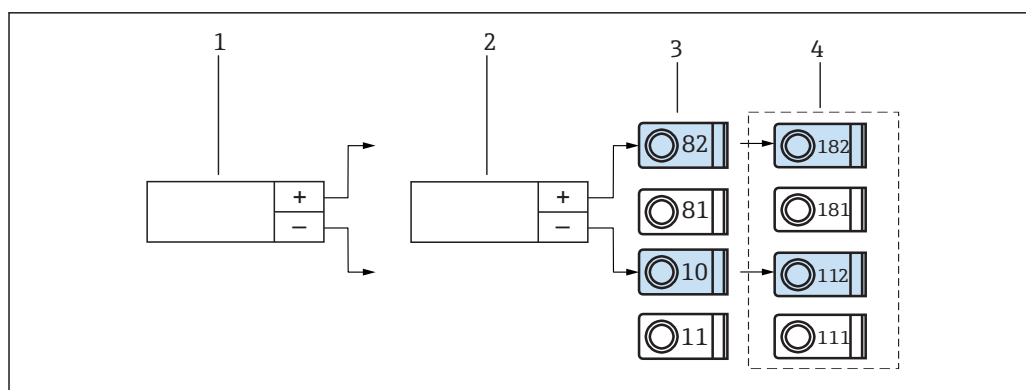


A0039673

10 Connection of the temperature sensor via the temperature head transmitter

- 1 TMT180 temperature sensor
- 2 TMT181 temperature head transmitter
- 3 Slot A I
- 4 Additional Slot B I

### Pressure sensor with passive current output

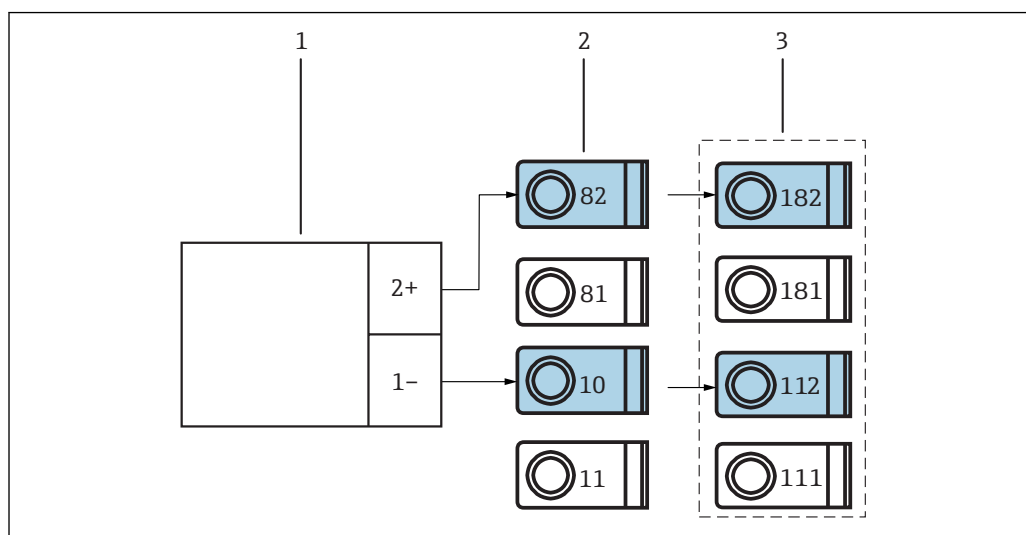


A0039674

11 Connection of the pressure sensor with passive current output

- 1 Cerabar S/M
- 2 Slot A I
- 3 Additional Slot B I

### Connecting outputs

The device has two galvanically isolated outputs or Ethernet connection, which can be configured as an analog output or active pulse output. In addition, an output for connecting a relay and the option of transmitter power supply are available for each device. The number of outputs increases according to the installed additional extension cards (→ 20).

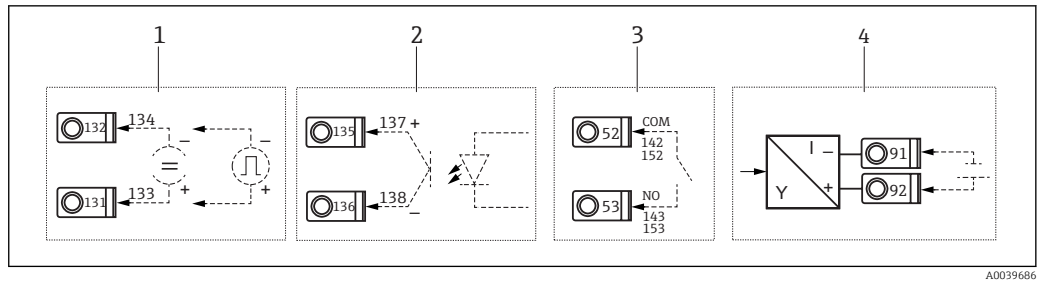


12 Connecting outputs

- 1 Active pulse and current outputs
- 2 Passive pulse output with the open collector
- 3 Relay output (NO), e.g. slot A III
- 4 Transmitter power supply (MUS) output

## Interface connection

### The bus interfaces:

- RS232  
The RS232 interface is connected via an interface cable and a jack socket on the front of the housing.
- RS485  
■ PROFIBUS®  
Optional connection of the Density Computer FML621 to PROFIBUS DP via the serial RS485 interface with the external module HMS AnyBus Communicator for PROFIBUS (→ 36).
- Optional interfaces:
  - additional RS485
  - Ethernet

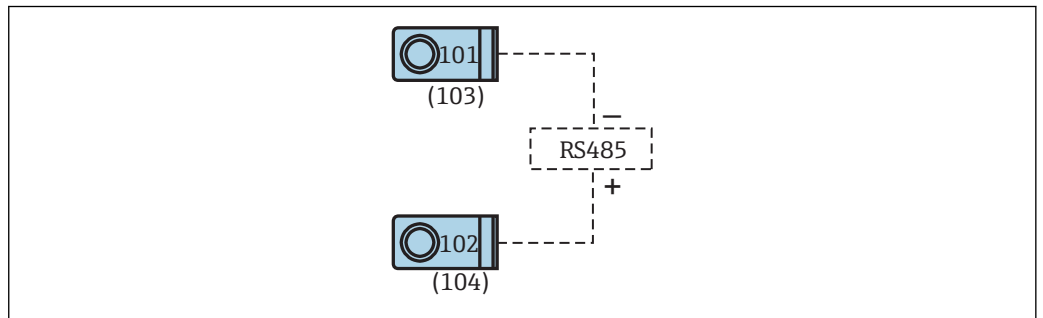


13 Interface connection

## Ethernet option

### Ethernet connection

An IEEE 802.3 compatible connection is available on a shielded RJ45 plug connector on the device underside as the network connection. This can be used to connect the device to devices in the office environment with a hub or switch. The office equipment standard EN 60950 must be taken into consideration for safe distances between equipment. The assignment corresponds to an MDI-interface (AT&T258) conforming to standards so that a shielded 1:1 cable with a maximum length of 100 m (328 ft) can be used. The Ethernet interface is designed as a 10 and 100-BASE-T. Direct connection to a PC is possible with a crossover cable. Half-duplex and full-duplex data transmission is supported.

- i** If the FML621 has an Ethernet interface, no analog outputs are available on the base unit via slot E!

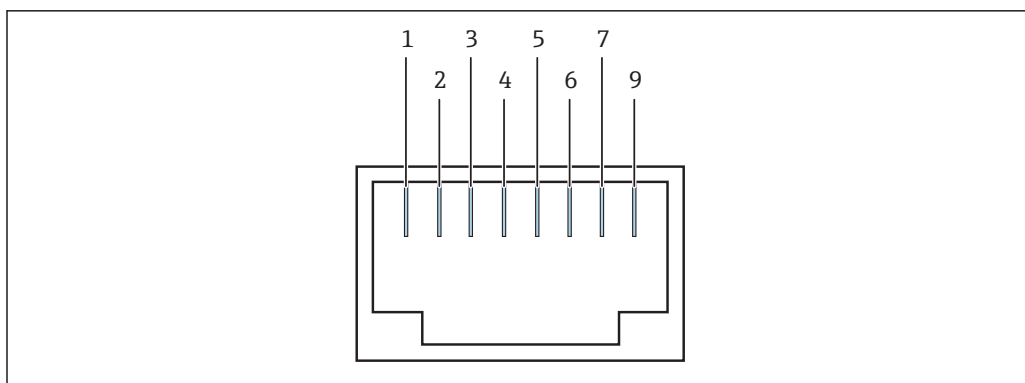

A0039690

14 RJ45 socket


- 1 Tx+
- 2 Tx-
- 3 Rx+
- 4 Not connected
- 5 Not connected
- 6 Rx-
- 7 Not connected
- 8 Not connected

### LED indicators

Two LEDs are located under the connector indicate the status of the Ethernet interface.

- yellow LED - link signal
  - lits when the device is connected to a network
- green LED - Tx/Rx
  - flashes when the device is sending or receiving data
  - lits constantly when the device is not sending or receiving data

### The extension cards

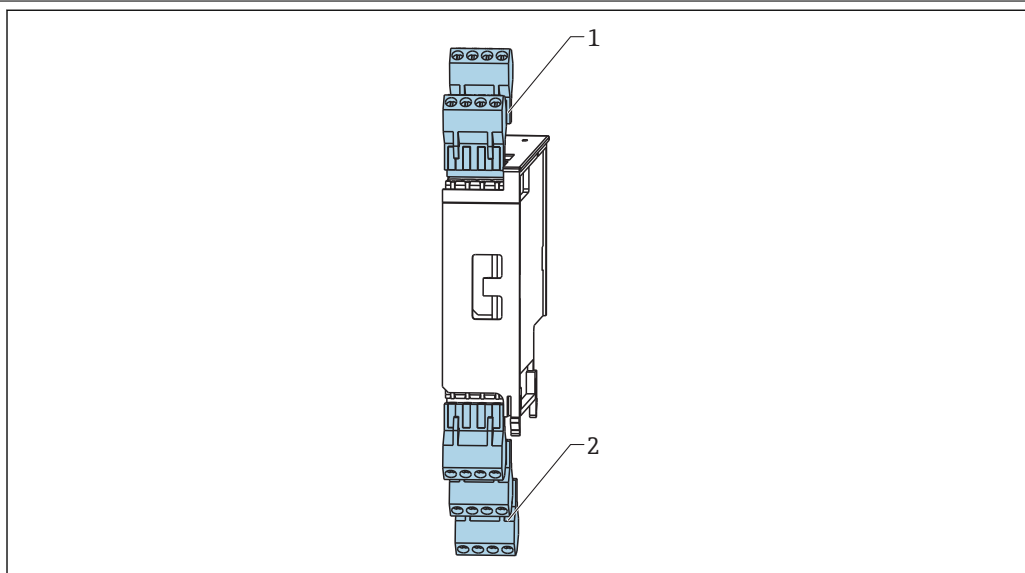

A0039691

15 Extension card with terminals

- 1 Input slots (I, II)
- 2 Outputs: (III, IV, V)

### Terminal assignment of "Universal extension card (FML621A-UA)" with intrinsically safe inputs (FML621A-UB)

#### Slot B I, C I, D I

Input: current or PFM or pulse input 1

- terminal 182: 24 V sensor power supply 1
- terminal 112: 0 to 20 mA or 4 to 20 mA, PFM, pulse input 1
- terminal 111: ground for 0 to 20 mA or 4 to 20 mA, PFM, pulse input
- terminal 181: sensor power supply ground 1

#### Slot B II, C II, D II

Input: current or PFM or pulse input 2

- terminal 183: 24 V sensor power supply 2
- terminal 181: sensor power supply ground 2
- terminal 113: 0 to 20 mA or 4 to 20 mA, PFM, pulse input 2
- terminal 111: ground for 0 to 20 mA or 4 to 20 mA, PFM, pulse input

#### Slot B III, C III, D III

Output: relay 1

- terminal 142: relay Common (COM)
- terminal 143: relay Normally Open (NO)
- Output: relay 2
- terminal 152: relay Common (COM)
- terminal 153: relay Normally Open (NO)

#### Slot B IV, C IV, D IV

Output: Current or pulse output - active

- terminal 131: + 0 to 20 mA or 4 to 20 mA pulse output 1
- terminal 132: - 0 to 20 mA or 4 to 20 mA pulse output 1
- terminal 133: + 0 to 20 mA or 4 to 20 mA pulse output 2
- terminal 134: - 0 to 20 mA or 4 to 20 mA pulse output 2

#### Slot B V, C V, D V


Output: Current or pulse output - passive


- terminal 135: + pulse output 3 - open collector
- terminal 136: - pulse output 3
- terminal 137: + pulse output 4 - open collector
- terminal 138: - pulse output 4


### Terminal assignment of "Temperature extension card (FML621A-TA)" with intrinsically safe inputs (FML621A-TB)

*Temperature sensors*

Connection for Pt100, Pt500 and Pt1000.

 Terminals 116 and 117 must be jumpered when connecting 3-wire sensors.

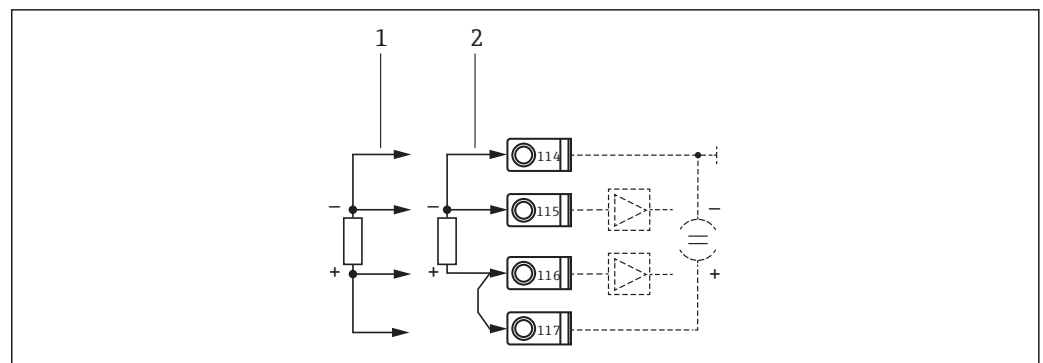

 16 Temperature sensor connection, optional temperature extension card e.g. in slot B (slot B I)

1 4-wire input

2 3-wire input

**Slot B I, C I, D I**

Input: RTD input 1

- terminal 117: + RTD power supply 1
- terminal 116: + RTD sensor 1
- terminal 115: - RTD sensor 1
- terminal 114: - RTD power supply 1

**Slot B II, C II, D II**

Input: RTD input 2

- terminal 121: + RTD power supply 1
- terminal 120: + RTD sensor 1
- terminal 119: - RTD sensor 1
- terminal 118: - RTD power supply 1

**Slot B III, C III, D III**

- output: Relay 1
  - terminal 142: relay 1 Common (COM)
  - terminal 143: relay 1 Normally Open (NO)
- output: Relay 2
  - terminal 152: relay 2 Common (COM)
  - terminal 153: relay 21 Normally Open (NO)

**Slot B IV, C IV, D IV**


- output: current or pulse 1 - active
  - terminal 131: + 0 to 20 mA or 4 to 20 mA
  - terminal 132: - 0 to 20 mA or 4 to 20 mA
- output: current or pulse 2 - active
  - terminal 133: + 0 to 20 mA or 4 to 20 mA
  - terminal 134: - 0 to 20 mA or 4 to 20 mA

**Slot B V, C V, D V**

- output: Passive pulse output
  - terminal 135: + pulse output 3 - open collector
  - terminal 136: - pulse output 3
- output: Passive pulse output
  - terminal 137: + pulse output 4 - open collector
  - terminal 138: - pulse output 4

**Terminal assignment of "Digital extension card (FML621A-DA)" with intrinsically safe inputs (FML621A-DB)**

The digital card has 6 intrinsically safe inputs. Terminals E1 and E4 can be defined as pulse inputs.

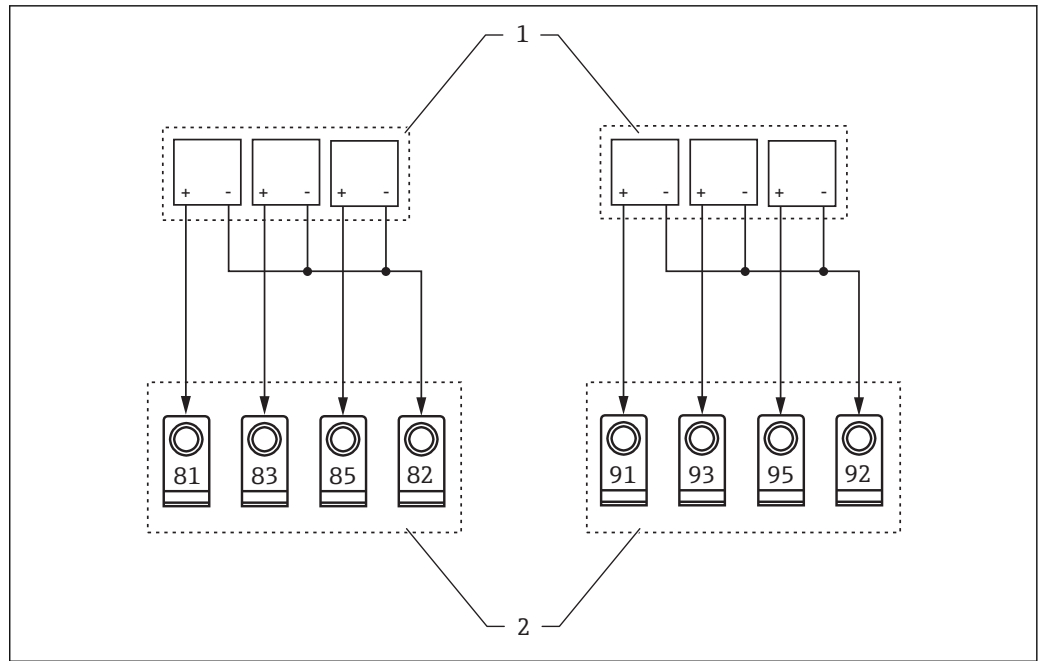

A0039694

17 Connecting the digital input

- 1 Digital input device  
2 Terminals

**i** The current, PFM, pulse inputs or the RTD inputs in the same slot are not galvanically isolated. There is a separation voltage of 500 V between the aforementioned inputs and outputs in various slots.

Terminals with the same second digit are jumpered internally.

#### Slots B I, C I, D I

Digital inputs E1 to 3

- terminal 81: E1 20 kHz or 4 Hz as pulse input
- terminal 83: E2 4 Hz
- terminal 85: E3 4 Hz
- terminal 82: Signal ground E1 to 3

#### Slots B II, C II, D II

Digital inputs E4 to 6

- terminal 91: E4 20 kHz or 4 Hz as pulse input
- terminal 93: E5 4 Hz
- terminal 95: E6 4 Hz
- terminal 92: Signal ground E4 to 6

#### Slots B III, C III, D III


- output: Relay 1
  - terminal 142: relay 1 Common (COM)
  - terminal 143: relay 1 Normally Open (NO)
- output: Relay 2
  - terminal 152: relay 2 Common (COM)
  - terminal 153: relay 2 Normally Open (NO)

#### Slots B IV, C IV, D IV

- output: Relay 3
  - terminal 145: relay 3 Common (COM)
  - terminal 146: relay 3 Normally Open (NO)
- output: Relay 4
  - terminal 155: relay 4 Common (COM)
  - terminal 156: relay 4 Normally Open (NO)

**Slots B V, C V, D V**

- output: Relay 5
  - terminal 242: relay 5 Common (COM)
  - terminal 243: relay 5 Normally Open (NO)
- output: Relay 6
  - terminal 252: relay 6 Common (COM)
  - terminal 253: relay 6 Normally Open (NO)

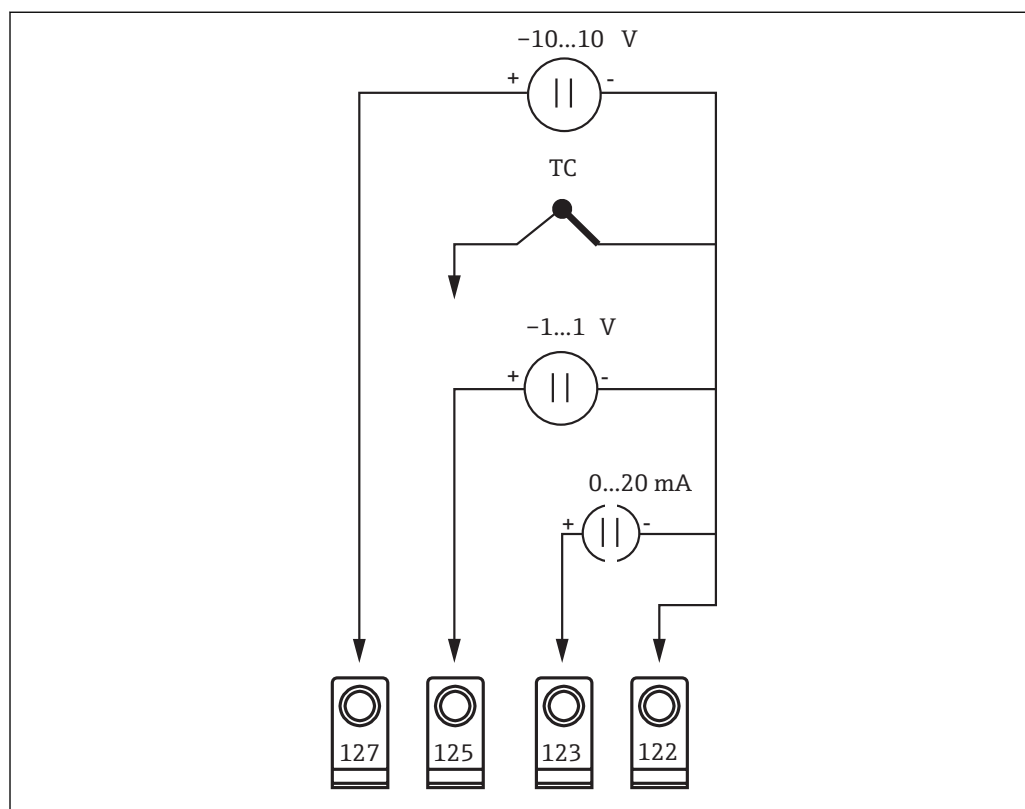**Terminal assignment of "U-I-TC extension card (FML621A-CA)" with intrinsically safe inputs (FML621A-CB)**


A0039695

18 U-I-TC card

**i** The card supports 2 input channels.

Channel 1 is supported by terminals 122, 123, 125 and 127.

Channel 2 is supported by terminals 222, 223, 225 and 227.

**Slots B I, C I, D I**
**U-I-TC Input 1**

- terminal 127: -10 to +10 V input
- terminal 125: -1 to +1 TC input
- terminal 123: 0 to 20 mA input
- terminal 122: Signal ground input

**Slots B II, C II, D II**
**U-I-TC Input 2**

- terminal 227: -10 to +10 V input
- terminal 225: -1 to +1 TC input
- terminal 223: 0 to 20 mA input
- terminal 222: Signal ground input



#### Slots B III, C III, D III

- output: Relay 1
  - terminal 142: relay 1 Common (COM)
  - terminal 143: relay 1 Normally Open (NO)
- output: Relay 2
  - terminal 152: relay 2 Common (COM)
  - terminal 153: relay 2 Normally Open (NO)

#### Slots B IV, C IV, D IV

- output: Current or pulse output 1 - active
  - terminal 131: + 0 to 20 mA or 4 to 20 mA or pulse output 1
  - terminal 132: - 0 to 20 mA or 4 to 20 mA or pulse output 1
- output: Current or pulse output 2 - active
  - terminal 133: + 0 to 20 mA or 4 to 20 mA or pulse output 2
  - terminal 134: - 0 to 20 mA or 4 to 20 mA or pulse output 2

#### Slot B V, C V, D V

- output: Passive pulse output
  - terminal 135: + pulse output 3 - open collector
  - terminal 136: - pulse output 3
- output: Passive pulse output
  - terminal 137: + pulse output 4 - open collector
  - terminal 138: - pulse output 4

### Connecting remote display unit and the operating unit

#### Functional description



#### Remember!

- connect the remote display unit to use all functions of the operation unit
- operation only with ReadWin® 2000 is not permitted
- connect only one display or operation unit to the top-hat rail device

The remote display is an innovative addition to the powerful FML621 top-hat rail device. The user has the opportunity to optimally install the arithmetic unit to suit the installation and mount the display and operating unit in a user-friendly way at easily accessible locations. The display can be connected to both a top-hat rail device without, as well as a top-hat rail device with, an integrated display or operating unit. A 4-pin cable is supplied to connect the remote display with the basic unit; other components are not necessary.

#### Installation of the remote display unit or operating unit




The place where the display unit is mounted must be free from vibrations.

The permitted ambient temperature during operation is  $-20$  to  $+60$  °C ( $-4$  to  $140$  °F).

Protect the device from exposure to high temperature or heat.

#### Installation of the display unit

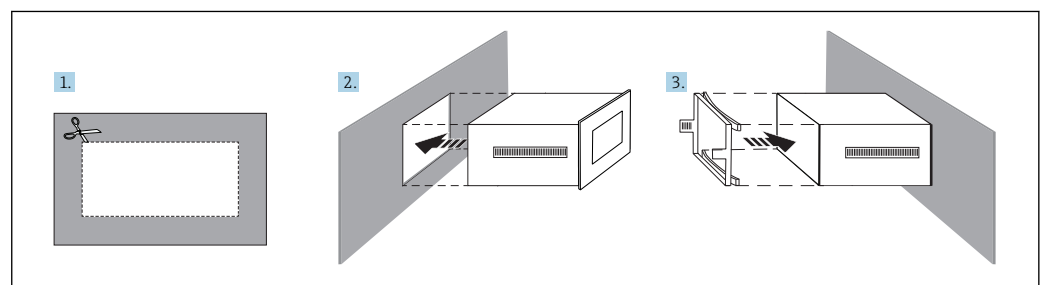

A0039697


#### 19 Installation of the display unit

##### 1 The display unit

1. Cut out a hole of dimensions: 138 mm (5.43 in) x 68 mm (2.68 in).
2. Push the device with the sealing ring through the hole from the front.
3. Push the secure frame over the rear of the housing against the panel until the retaining clips engage.
  - ↳ The display unit is mounted.

## Wiring

The remote display unit and operating unit are connected directly to the basic unit with the supplied cable.

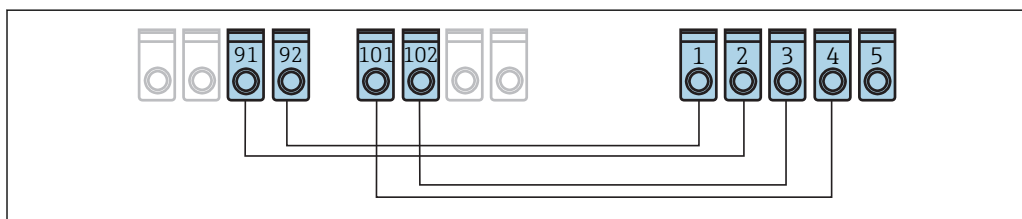

A0039699

20 Wire connections between remote display unit and base unit.

- 1 Terminal GDN - remote display unit
- 2 Terminal 24 V<sub>DC</sub> - remote display unit
- 3 Terminal + Rx Tx - remote display unit
- 4 Terminal - Rx Tx - remote display unit
- 5 Terminal PE - remote display unit
- 91 Terminal GND - Slot A III - base unit
- 92 Terminal 24 V<sub>DC</sub> - Slot A III - base unit
- 101 Terminal - Rx Tx - Slot E III - base unit
- 102 Terminal + Rx Tx - Slot E III - base unit

## Post-connection check

After completing the electrical installation of the device, carry out the following checks:

☐ Do a visual inspection that the cable is not damaged.

Contact E+H Service directly when the device is incomplete or damaged.

☐ Check the power supply voltage. The voltage must be same as shown on the name plate.

The power supply voltage parameters are:

90 to 250 V<sub>AC</sub> 50 to 60 Hz

20 to 28 V<sub>AC</sub> 50 to 60 Hz

18 to 36 V<sub>DC</sub>

☐ Check the power supply and signal cables are connected correctly.

Compare the wiring diagram with the connections in the terminals.

☐ Check the terminals coding.

☐ Check that the terminal slot is inserted correctly.

☐ Check that the cables are not tensioned.

## Power supply

### Supply voltage

- low voltage power unit: 90 to 230 V<sub>AC</sub> 50 to 60 Hz
- extra-low voltage power unit: 20 to 36 V<sub>DC</sub> or 20 to 28 V<sub>AC</sub> 50 to 60 Hz

### Power consumption

8 to 38 VA - depending to version and wiring.

### Connection data interface

#### RS232

- connection: jack socket 3.5 mm (0.14 in), front
- transmission protocol: ReadWin® 2000
- transmission rate: max. 57 600 baud

#### RS485

- connection: plug-in terminals 101 and 102
- transmission protocol:
  - serial: ReadWin® 2000
  - parallel: open standard
- transmission rate: max. 57 600 baud

**Optional: additional RS485 interface**

- connection: plug-in terminals 103 and 104
- transmission protocol and transmission rate as standard interface RS485

**Optional: Ethernet interface**

- Ethernet interface: 10/100 BaseT
- connector type: RJ45
- connection via shielded cable
- issuing of IP address via setup menu in the device

Connection by interface with devices is possible only in office environment.

Safety distances: office device standard IEC 60950-1 must be taken into consideration.

Connection to a PC is possible via "crossover" cable.

## Reference operating conditions

**FML621 reference operating conditions**

- power supply: 207 to 250 V<sub>AC</sub> ±10 %, 50 Hz, ±0.5 Hz
- warm-up period: >30 min
- ambient temperature: 25 °C (77 °F), ±5 °C (±9 °F)
- air humidity: 39 % ±10 % r.h.

**Reference operating conditions for special calibration and Liquiphant M Density**

- medium: water H<sub>2</sub>O
- medium temperature: 0 to 80 °C (32 to 176 °F), liquid not moved
- ambient temperature: 24 °C (75 °F) ±5 °C (±9 °F)
- humidity: max. 90 %
- warm-up period: >30 min

## Performance characteristics



The accuracy described here refers to the entire density measuring line.

**General measuring conditions for accuracy data**

- measuring range: 300 to 2 000 kg/m<sup>3</sup> (18.7 to 124.9 lb/ft<sup>3</sup>)
- distance between paddle and container wall and surface of liquid: > 50 mm (1.97 in)
- temperature sensor measured error: < 1 K
- maximum viscosity: 350 mPa·s (3.5 P)
- maximum flow velocity: 2 m/s (6.56 ft/s)
  - laminar flow, bubble-free (→ 29)
  - construction-specific measures like bypass or pipe enlargement for reduction must be put in place for higher flow velocities
- process temperature: 0 to +80 °C (32 to 176 °F) - validity of accuracy data
- power supply in accordance with specification FML621
- information in accordance with DIN EN 61298-2
- process pressure: -1 to 25 bar (-14.5 to 362.5 psi)

**Maximum measured error**

- 1 g/cm<sup>3</sup> = 1 SGU (Specific Gravity Unit)
- standard adjustment: ±0.02 g/cm<sup>3</sup> (±1.2 % of the span 1.7 g/cm<sup>3</sup>, under general measuring conditions)
  - special adjustment: ±0.005 g/cm<sup>3</sup> (±0.3 % of the span 1.7 g/cm<sup>3</sup>, under reference operating conditions)
  - field adjustment: ±0.002 g/cm<sup>3</sup> (in operating point)

**Non-repeatability - reproducibility**

- 1 g/cm<sup>3</sup> = 1 SGU (Specific Gravity Unit)
- standard adjustment: ±0.002 g/cm<sup>3</sup> (under general measuring conditions)
  - special adjustment: ±0.0007 g/cm<sup>3</sup> (under reference operating conditions)
  - field adjustment: ±0.002 g/cm<sup>3</sup> (in operating point)

**Factors influencing accuracy data**

- clean the sensor (CIP or SIP) at process temperatures of up to 140 °C (284 °F) over a long period
- all information on the accuracy of measuring viscosity of liquids refers to Newtonian liquids
- it is not possible to perform density measurement in liquids: gel, viscoelastic gel, non-Newtonian elastic, pseudoelastic and plastic-viscous liquids.
- long-term drift typ.: 0.02 kg/m<sup>3</sup> (0.001 lb/ft<sup>3</sup>) per day
- temperature coefficient typ.: ±0.2 kg/m<sup>3</sup> (±0.01 lb/ft<sup>3</sup>) per 10 K
- fluid velocity in pipes: >2 m/s (6.56 ft/s)
- buildup at the fork
- air bubbles in the case of vacuum applications
- incomplete coverage of the fork
- for pressure changes >6 bar (87 psi), a pressure measurement is required for compensation
- for temperature changes >1 K, a temperature measurement is required for compensation
- mechanical stress, e.g. deformation on the fork tines can impact accuracy and must be avoided
- the device subjected to mechanical stress must be replaced

Cyclic field adjustment can take place depending on the accuracy required.

## FML621 installation instructions

**Mounting location** Mount the device in a cabinet on top-hat rail IEC 60715.

**Orientation** No restrictions.

## Environment

**Ambient temperature range**

**Extension cards generate extra heat.**

Destruction of electronic components.

- Install an additional ventilation with a minimum air flow rate of 0.5 m/s (1.64 ft/s).

Temperature range: -20 to 50 °C (-4 to 122 °F).

**Storage temperature** -30 to 70 °C (-22 to 158 °F)

**Climate class** As per IEC 60654-1 Class B2 / EN 1434 Class "C" - no condensation permitted.

**Electrical safety** As per IEC 61010-1: environment <2 000 m (6 560 ft) height above sea level.

**Degree of protection**

- basic unit: IP 20
- remote operating and display unit: front IP 65

**Electromagnetic compatibility****Interference emission**

IEC 61326 Class A

**Interference immunity**

- power failure: 20 ms, no influence
- starting current limitation:  $I_{\max}/I_n < 50\%$  ( $T 50\% \leq 50$  ms)
- electromagnetic fields: 10 V/m (3.048 V/ft) as per IEC 61000-4-3
- conducted HF: 0.15 to 80 Hz, 10 V/10 V to IEC 61000-4-3
- electrostatic discharge: 6 kV contact, indirect as per IEC 61000-4-2
  - burst - power supply: 2 kV as per IEC 61000-4-4
  - burst - signal: 1 kV/2 kV as per IEC 61000-4-4
  - surge - power supply AC: 1 kV/2 kV as per IEC 61000-4-5
  - surge - power supply DC: 1 kV/2 kV as per IEC 61000-4-5
  - surge - signal: 0.5 kV/1 kV as per IEC 61000-4-5


## Installation conditions for Liquiphant



The following information is supplemented by additional documentation on Liquiphant (→ 37).

### Orientation

The mounting location must be selected such that the fork tines and the diaphragm are always immersed in the medium.

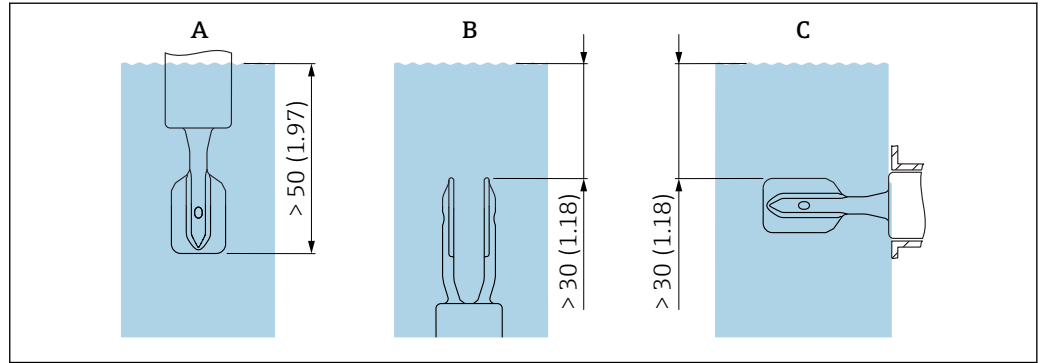

21 Unit of measurement mm (in)

- A Top installation
- B Bottom installation
- C Side installation


### Inlet and outlet run

#### Inlet run

Install the sensor as far as possible from fittings such as: valves, T-sections, elbows, flange elbows, etc.

Compliance with the following requirements for the inlet run is necessary in order to ensure measuring accuracy:

Inlet run:  $\geq 5 \times \text{ND}$  (nominal diameter) - min. 750 mm (29.5 in)

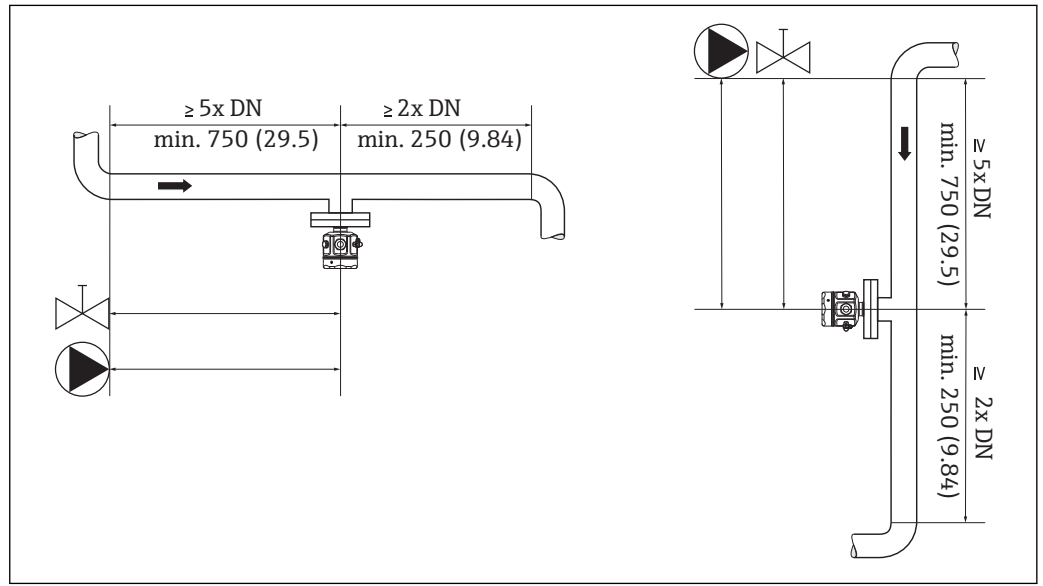


22 Inlet run installation

#### Outlet run

Compliance with the following requirements for the outlet run is necessary in order to ensure measuring accuracy:

Outlet run:  $\geq 2 \times \text{ND}$  (nominal diameter) - min. 250 mm (9.84 in)

Pressure and temperature sensor must be installed downstream from the flow direction of the Liquiphant Density. When installing pressure and temperature measuring points downstream of the measuring device, make sure the distance between the measuring point and the measuring device is sufficient.

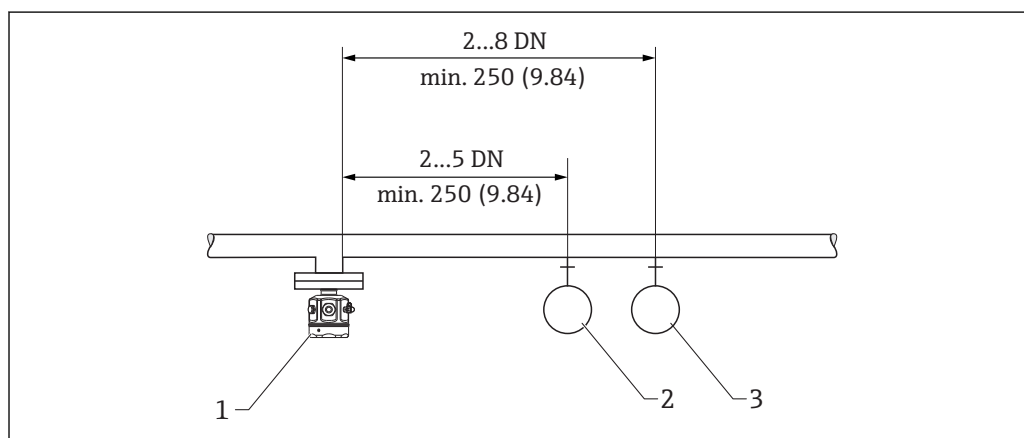

A0039701

23 Outlet run installation

- 1 Liquiphant sensor
- 2 Pressure measuring point
- 3 Temperature measuring point

#### Mounting location and correction factor

The Liquiphant can be installed in containers, tanks or pipes.

#### Correction factor "r"

The vibrating fork tines of the Liquiphant Density device need free space to vibrate. The medium has to flow around the fork tines. The measurement result is affected if the distance between the fork tines and the tank or pipe wall is very small. The measurement error can be balanced by entering a correction factor "r".


	h	r
<p>Unit of measurement mm (in)</p>	12 mm (0.47 in)	1,0026
	14 mm (0.55 in)	1,0016
	16 mm (0.63 in)	1,0011
	18 mm (0.71 in)	1,0008
	20 mm (0.79 in)	1,0006
	22 mm (0.87 in)	1,0005
	24 mm (0.94 in)	1,0004
	26 mm (1.02 in)	1,0004
	28 mm (1.10 in)	1,0004
	30 mm (1.18 in)	1,0003
	32 mm (1.26 in)	1,0003
	34 mm (1.34 in)	1,0002
	36 mm (1.42 in)	1,0001
	38 mm (1.50 in)	1,0001
	40 mm (1.57 in)	1,0001

A0039687

In pipe internal fittings, the fork tines of the Liquiphant must be aligned with the direction of flow. Otherwise, the measurement result can be distorted by vortexes and eddies.


- A mark on the process connection indicates the position of the fork tines.  
Threaded connection = dot on the hexagon head; flange = two lines on the flange.
- The flow velocity of the medium may not exceed 2 m/s (6.56 ft/s) during the operation

In tanks with an agitator, the Liquiphant must be aligned in the direction of flow. Otherwise, the measurement result can be distorted by vortexes and eddies.

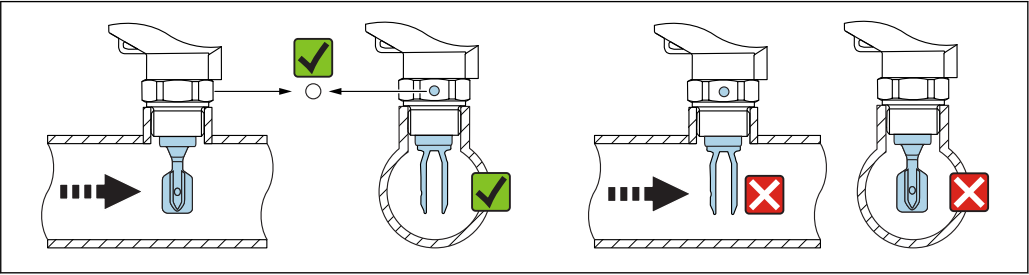

A0034851

24 Fork position and marking


	D	r
 <i>Unit of measurement mm (in)</i>	<44 mm (1.73 in)	-
	44 mm (1.73 in)	1,0225
	46 mm (1.81 in)	1,0167
	48 mm (1.89 in)	1,0125
	50 mm (1.97 in)	1,0096
	52 mm (2.05 in)	1,0075
	54 mm (2.13 in)	1,0061
	56 mm (2.20 in)	1,0051
	58 mm (2.28 in)	1,0044
	60 mm (2.36 in)	1,0039
	62 mm (2.44 in)	1,0035
	64 mm (2.52 in)	1,0032
	66 mm (2.60 in)	1,0028
	68 mm (2.68 in)	1,0025
	70 mm (2.76 in)	1,0022
	72 mm (2.83 in)	1,0020
	74 mm (2.91 in)	1,0017
	76 mm (2.99 in)	1,0015
	78 mm (3.07 in)	1,0012
	80 mm (3.15 in)	1,0009
	82 mm (3.23 in)	1,0007
	84 mm (3.31 in)	1,0005
	86 mm (3.39 in)	1,0004
	88 mm (3.46 in)	1,0003
	90 mm (3.54 in)	1,0002
	92 mm (3.62 in)	1,0002
	94 mm (3.70 in)	1,0001
	96 mm (3.78 in)	1,0001
	98 mm (3.86 in)	1,0001

A0039707

	D	r
	100 mm (3.94 in)	1,0001
	>100 mm (3.94 in)	1,0000


**i** Pipe nominal diameters with internal measurements <44 mm (1.73 in) is not permitted!

If the flow in the pipes is strong, 2 to 5 m/s (6.56 to 16.4 ft/s), or in the event of turbulent surfaces in tanks, construction specific measures for the reduction of the turbulence at the sensor must be put in place. The Liquiphant Density can be installed in a bypass or in a pipe with a larger diameter for this purpose.

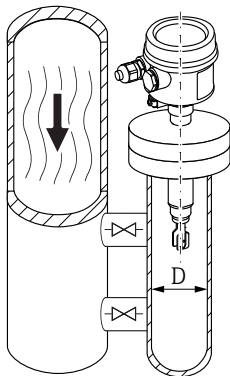	D	r
 <p>Unit of measurement mm (in)</p> <p>A0039689</p>	<44 mm (1.73 in)	-
	44 mm (1.73 in)	1,0191
	46 mm (1.81 in)	1,0162
	48 mm (1.89 in)	1,0137
	50 mm (1.97 in)	1,0116
	52 mm (2.05 in)	1,0098
	54 mm (2.13 in)	1,0083
	56 mm (2.20 in)	1,0070
	58 mm (2.28 in)	1,0059
	60 mm (2.36 in)	1,0050
	62 mm (2.44 in)	1,0042
	64 mm (2.52 in)	1,0035
	66 mm (2.60 in)	1,0030
	68 mm (2.68 in)	1,0025
	70 mm (2.76 in)	1,0021
	72 mm (2.83 in)	1,0017
	74 mm (2.91 in)	1,0014
	76 mm (2.99 in)	1,0012
	78 mm (3.07 in)	1,0010
	80 mm (3.15 in)	1,0008
	82 mm (3.23 in)	1,0006
	84 mm (3.31 in)	1,0005
	86 mm (3.39 in)	1,0004
	88 mm (3.46 in)	1,0003
	90 mm (3.54 in)	1,0003
	92 mm (3.62 in)	1,0002
	94 mm (3.70 in)	1,0002
	96 mm (3.78 in)	1,0001
	98 mm (3.86 in)	1,0001
	100 mm (3.94 in)	1,0001
	>100 mm (3.94 in)	1,0000





## Ambient conditions for Liquiphant Density


Ambient temperature range	-40 to 70 °C (-40 to 158 °F)
	 For further information on use in hazardous areas (ATEX) (→  37).

## Mechanical construction

Terminals	Pluggable screw terminals - power supply terminal coded. The clamping area 1.5 mm <sup>2</sup> (16 AWG) solid, 1 mm <sup>2</sup> (18 AWG) flexible with ferrules - applies to all connections.
-----------	--

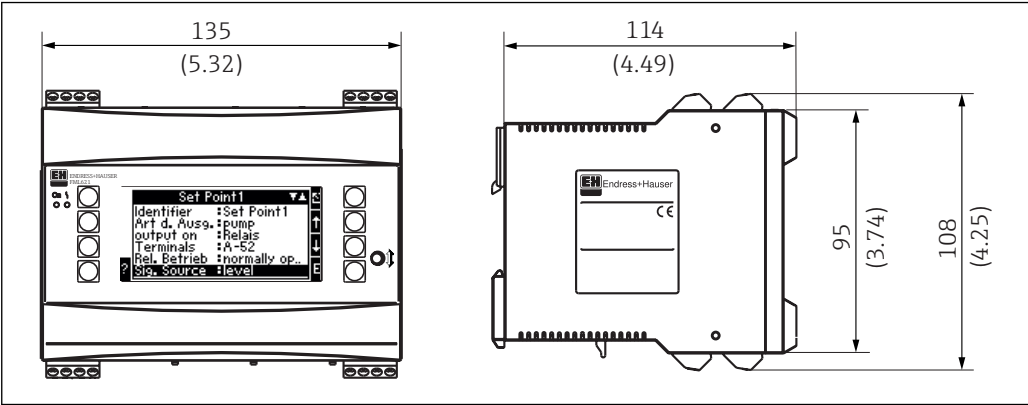Design	<div>Dimensions</div> <div><p>The technical drawing shows two views of the FML621 housing. The front view on the left indicates a width of 135 mm (5.32 inches). The side view on the right indicates a depth of 114 mm (4.49 inches). The side view also shows two height dimensions: 95 mm (3.74 inches) for the main body and 108 mm (4.25 inches) for the total height including the top rail. The front view shows a central LCD screen displaying 'Set Point1' and various parameters like 'Identifier', 'Art d. Ausg.', 'output on', 'Terminals', 'Rel. Betrieb', and 'Sig. Source'. The side view shows the 'Endress+Hauser' logo and a 'CE' mark.</p></div>
--------	---

 25 Housing for top-hat rail as per IEC 60715

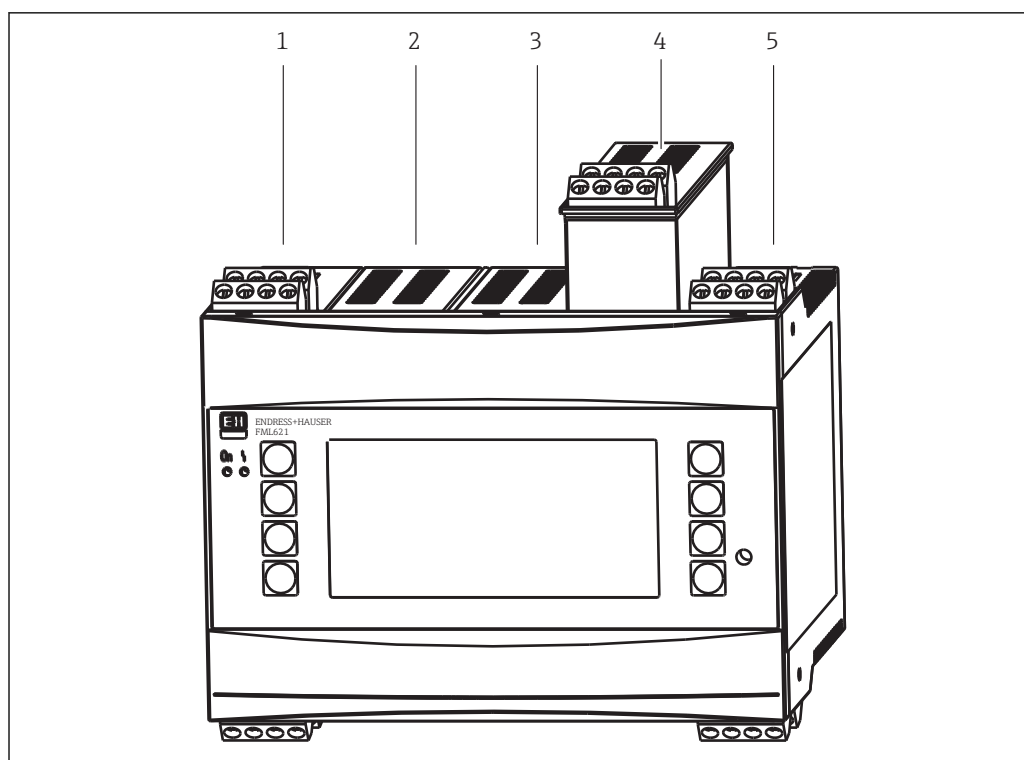

A0039710

26 The device with additional extension cards

- 1 Slot A
- 2 Slot B - an extension card
- 3 Slot C - an extension card
- 4 Slot D - an extension card
- 5 Slot E

### Weight

#### Basic unit:

500 g (17.6 oz). Weight with all additional extension cards.

#### Remote operating unit:

300 g (10.6 oz).

### Material

#### Housing:

Polycarbonate plastic, UL 94V0.

## Display and operating elements

- i** an operating and display unit is absolutely essential for field adjustment.
- an operating and display unit can also be used for commissioning Density Computer FML621.
- the operating and display unit can also be used for a number of devices.

### Display elements

#### Display


160x80 DOT matrix LCD with blue background lighting. The background light color changes to red in the event of an error. The background color is configurable.

#### LED status display

- operation: 1x green 2 mm (0.08 in)
- fault message: 1x red 2 mm (0.08 in)


### Operating and display unit - optional or as accessory

- an operating and display unit can be additionally connected to the device in the panel mounting housing with dimensions:
  - W: 144 mm (5.67 in)
  - H: 72 mm (2.83 in)
  - D: 43 mm (1.69 in)
- the connection to the integrated RS484 interface is made using the connecting cable, length = 3 m (9.84 ft) is included in the accessories kit
- parallel operation of the operating and display unit with a device-internal display in the FML621 is possible

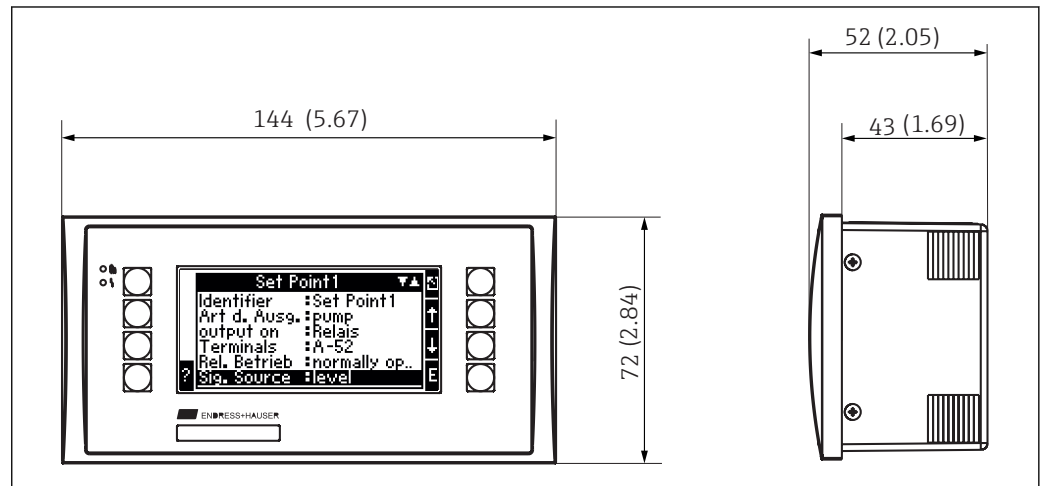

A0039711

27 Operating and display unit for panel mounting

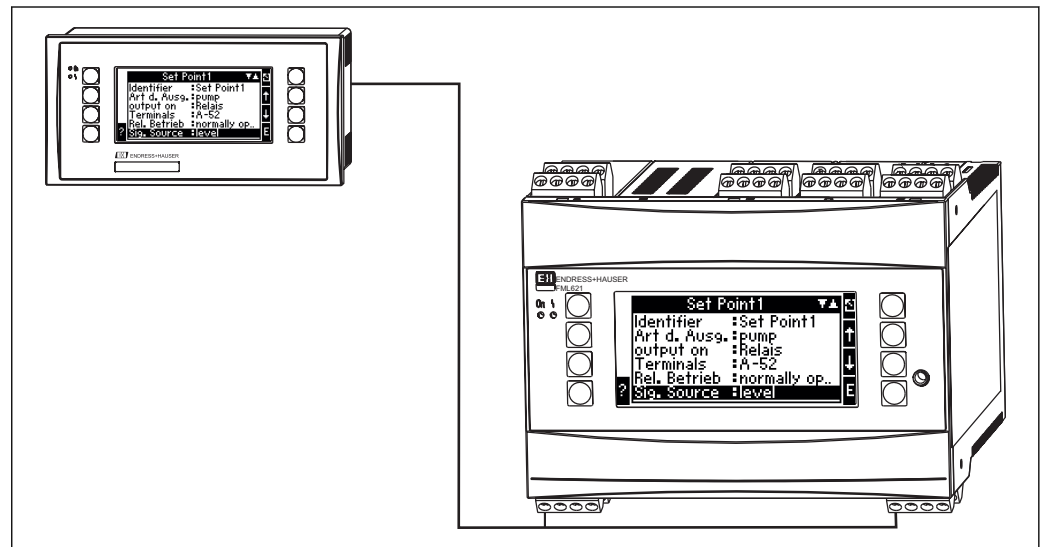

A0039717

28 Operating and display unit in panel mounting housing

- 1 Operating or display unit
- 2 Base unit

### Operating elements

Eight front-panel soft keys interact with the display. The key functions are shown on the display.

### Remote operation

- RS232 interface via mini jack socket 3.5 mm (0.14 in), configuration using PC and software ReadWin® 2000 PC
- RS485 interface

### Real time clock

- deviation: 30 min per year
- power reserve: 14 days

## Certificates and approvals

<b>CE mark</b>	<p>The measuring system meets the legal requirements of the applicable EC guidelines. These are listed in the corresponding EC Declaration of Conformity together with the standards applied.</p> <p>Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.</p>
<b>Ex approval</b>	<p>Available Ex approvals: see Product Configurator</p> <p>All explosion protection data are given in a separate documentation available on demand.</p>
<b>Other standards and guidelines</b>	<p><b>IEC 60529</b> Degrees of protection provided by enclosures (IP code)</p> <p><b>IEC 61010</b> Protection measures for electrical equipment for measurement, control, regulation and laboratory procedures</p> <p><b>EN 61326 series</b> EMC product family standard for electrical equipment for measurement, control and laboratory use</p> <p><b>NAMUR</b> User association of automation technology in process industries</p>

## Ordering information

Detailed ordering information is available from the following sources:

- in the *Product Configurator* on the Endress+Hauser website: [www.endress.com](http://www.endress.com) -> Click *Corporate* -> Select your country -> Click *Products* -> Select the product using the filters and search field -> Open product page -> The *Configure* button to the right of the product image opens the Product Configurator.
- from your Endress+Hauser Sales Center: [www.addresses.endress.com](http://www.addresses.endress.com).



Product Configurator - the tool for individual product configuration

- up-to-the-minute configuration data
- depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
- automatic verification of exclusion criteria
- automatic creation of the order code and its breakdown in PDF or Excel output format
- ability to order directly in the Endress+Hauser Online Shop

## Accessories

<b>General</b>	<p><b>RXU10-A1</b> Cable set for FML621 for connecting to a PC or modem</p> <p><b>FML621A-AA</b> Remote display for panel mounting:</p> <ul style="list-style-type: none"> <li>■ W: 144 mm (5.67 in)</li> <li>■ H: 72 mm (2.83 in)</li> <li>■ D: 43 mm (1.69 in)</li> </ul> <p><b>RMS621A-P1</b> PROFIBUS Interface</p> <p><b>51004148</b> Adhesive label, printed, max. 2x 16 characters</p> <p><b>51002393</b> Metal plate for TAG number</p> <p><b>51010487</b> Plate, paper, TAG 3x 16 characters</p>
----------------	---

<b>Extension cards</b>	<p>The device can be extended with a maximum of 3 universal or digital or current or Pt100 cards.</p> <p><b>FML621A-DA</b> Digital</p> <ul style="list-style-type: none"> <li>■ 6x digital input</li> <li>■ 6x relay output</li> <li>■ kit including terminals and fixing frame</li> </ul> <p><b>FML621A-DB</b> Digital, ATEX approved</p> <ul style="list-style-type: none"> <li>■ 6x digital input</li> <li>■ 6x relay output</li> <li>■ kit including terminals</li> </ul> <p><b>FML621A-CA</b> 2x U, I, TC</p> <ul style="list-style-type: none"> <li>■ 2x 0 to 20 mA or 4 to 20 mA per pulse</li> <li>■ 2x digital</li> <li>■ 2x relay SPST</li> </ul> <p><b>FML621A-CB</b> Multifunction, 2x U, I, TC ATEX</p> <ul style="list-style-type: none"> <li>■ 2x 0 to 20 mA or 4 to 20 mA per pulse</li> <li>■ 2x digital</li> <li>■ 2x relay SPST</li> </ul> <p><b>FML621A-TA</b> Temperature (Pt100/Pt500/Pt1000) complete, including terminals and fixing frame</p> <p><b>FML621A-TB</b> Temperature, ATEX approved (Pt100/PT500/PT1000) complete, including terminals</p> <p><b>FML621A-UA</b> Universal - PFM or pulse or analog or transmitter power supply unit complete, incl. terminals and fixing frame</p> <p><b>FML621A-UB</b> Universal ATEX approved - PFM or pulse or analog or transmitter power supply unit complete, including terminals</p>
------------------------	--

## Documentation

The following documentation types are available in the Downloads of the Endress+Hauser website ([www.endress.com/downloads](http://www.endress.com/downloads)):



For an overview of the scope of the associated Technical Documentation, refer to the following:

- *W@M Device Viewer* ([www.endress.com/deviceviewer](http://www.endress.com/deviceviewer)): Enter the serial number from nameplate
- *Endress+Hauser Operations App*: Enter the serial number from the nameplate or scan the 2D matrix code (QR code) on the nameplate

<b>Brief Operating Instructions (KA)</b>	<p><b>Guide that takes you quickly to the 1st measured value</b></p> <p>The Brief Operating Instructions contain all the essential information from incoming acceptance to initial commissioning.</p>
<b>Operating Instructions (BA)</b>	<p><b>Your reference guide</b></p> <p>These Operating Instructions contain all the information that is required in various phases of the life cycle of the device: from product identification, incoming acceptance and storage, to mounting, connection, operation and commissioning through to troubleshooting, maintenance and disposal.</p>
<b>Safety Instructions (XA)</b>	<p>Depending on the approval, the following Safety Instructions (XA) are supplied with the device. They are an integral part of the Operating Instructions.</p> <p> The nameplate indicates the Safety Instructions (XA) that are relevant to the device.</p>

---

---

[www.addresses.endress.com](http://www.addresses.endress.com)

---